
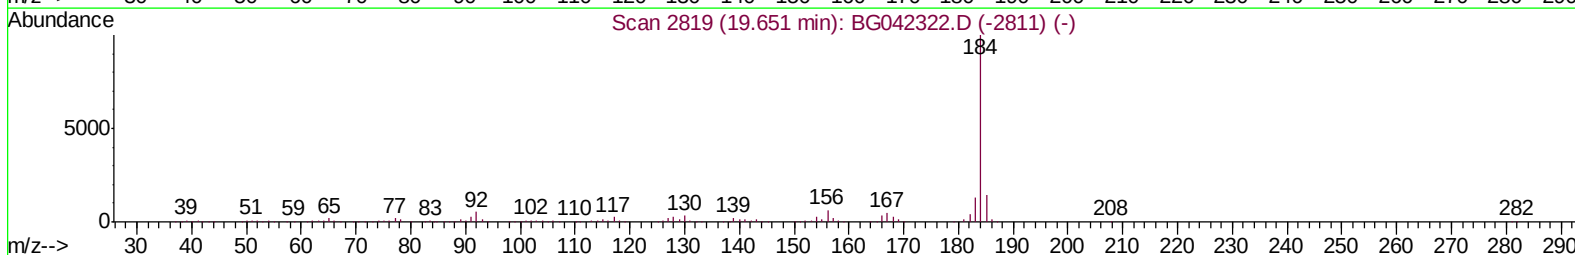
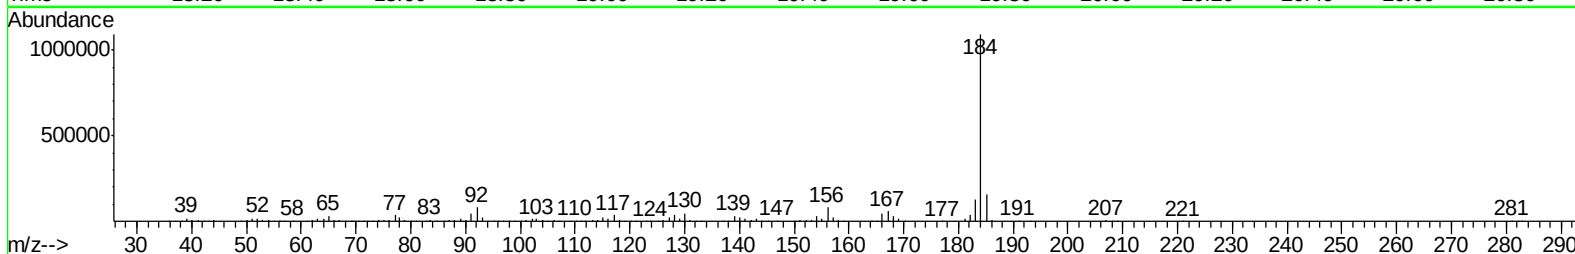


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082119\
Data File : BN007283.D
Acq On : 21 Aug 2019 08:27
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:27:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG081919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 13:40:37 2019
Response via : Initial Calibration

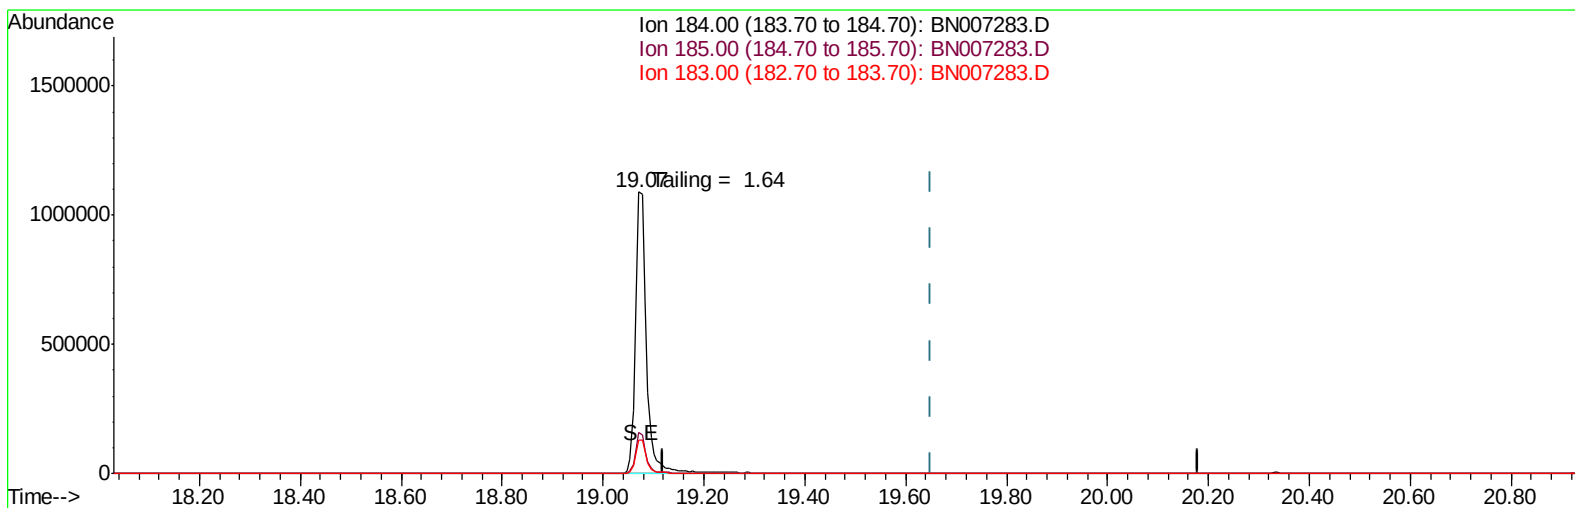

TIC: BN007283.D

(77) Benzidine




19.072min (-0.579) 134168.00ng

response 1647036

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.49
183.00	13.20	11.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN082119\
Data File : BN007283.D
Acq On : 21 Aug 2019 08:27
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 21 18:27:55 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG081919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 19 13:40:37 2019
Response via : Initial Calibration

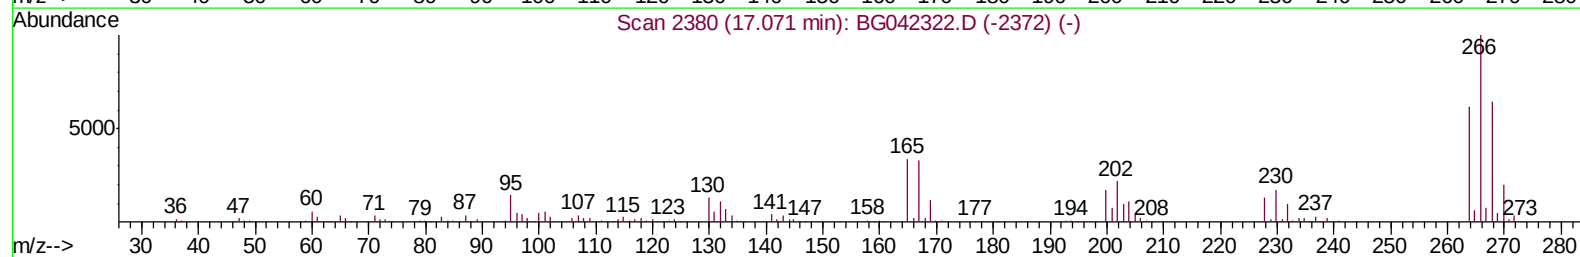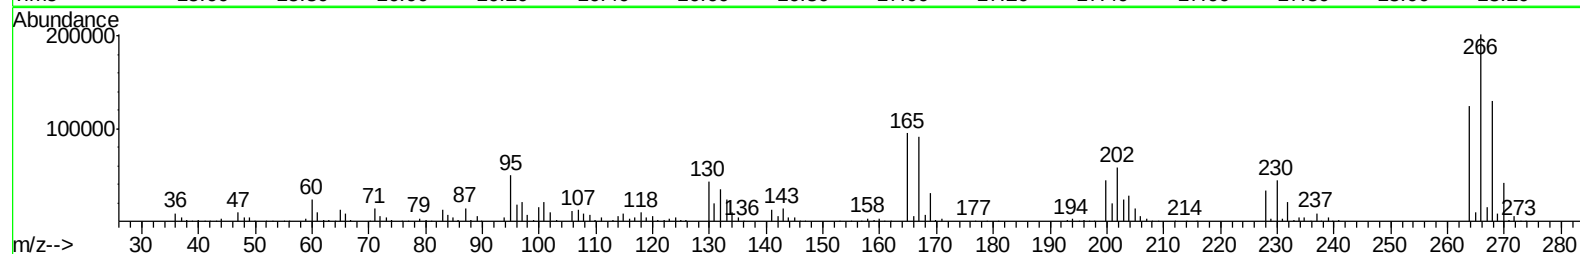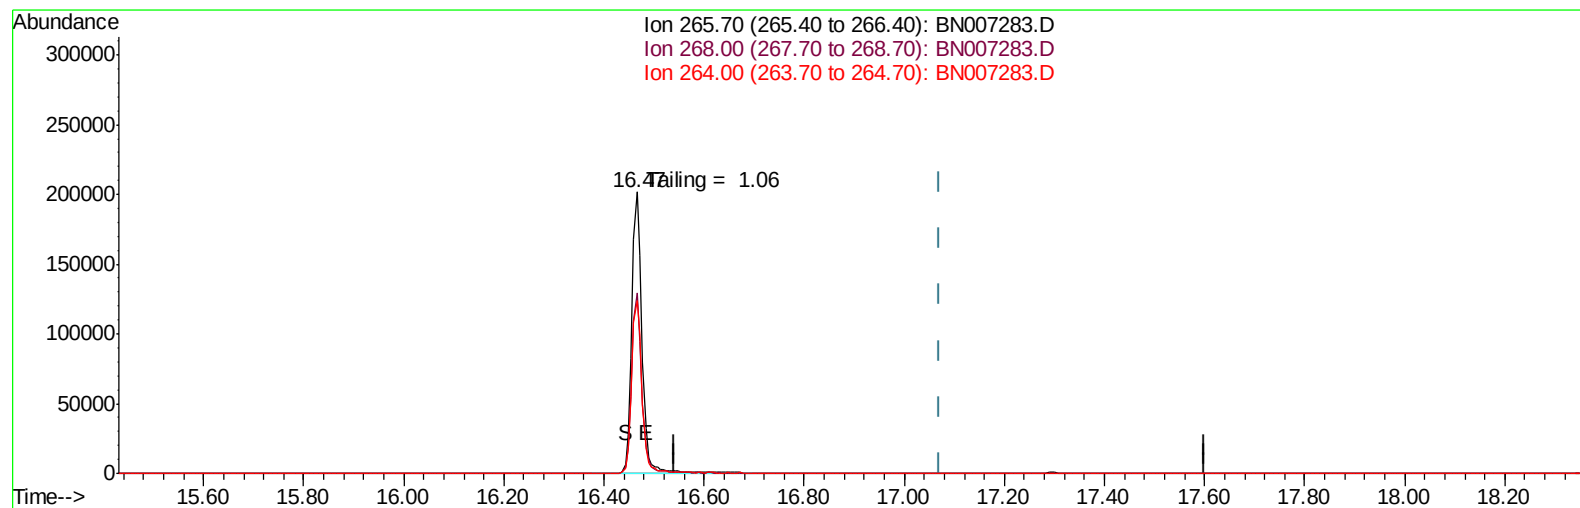

TIC: BN007283.D

(70) Pentachlorophenol (C)

16.466min (-0.606) 24448.66ng

response 283322

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	64.25
264.00	61.90	61.47
0.00	0.00	0.00