


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN082119\
 Data File : BN007283.D
 Acq On : 21 Aug 2019 08:27
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 18:52:43 2019

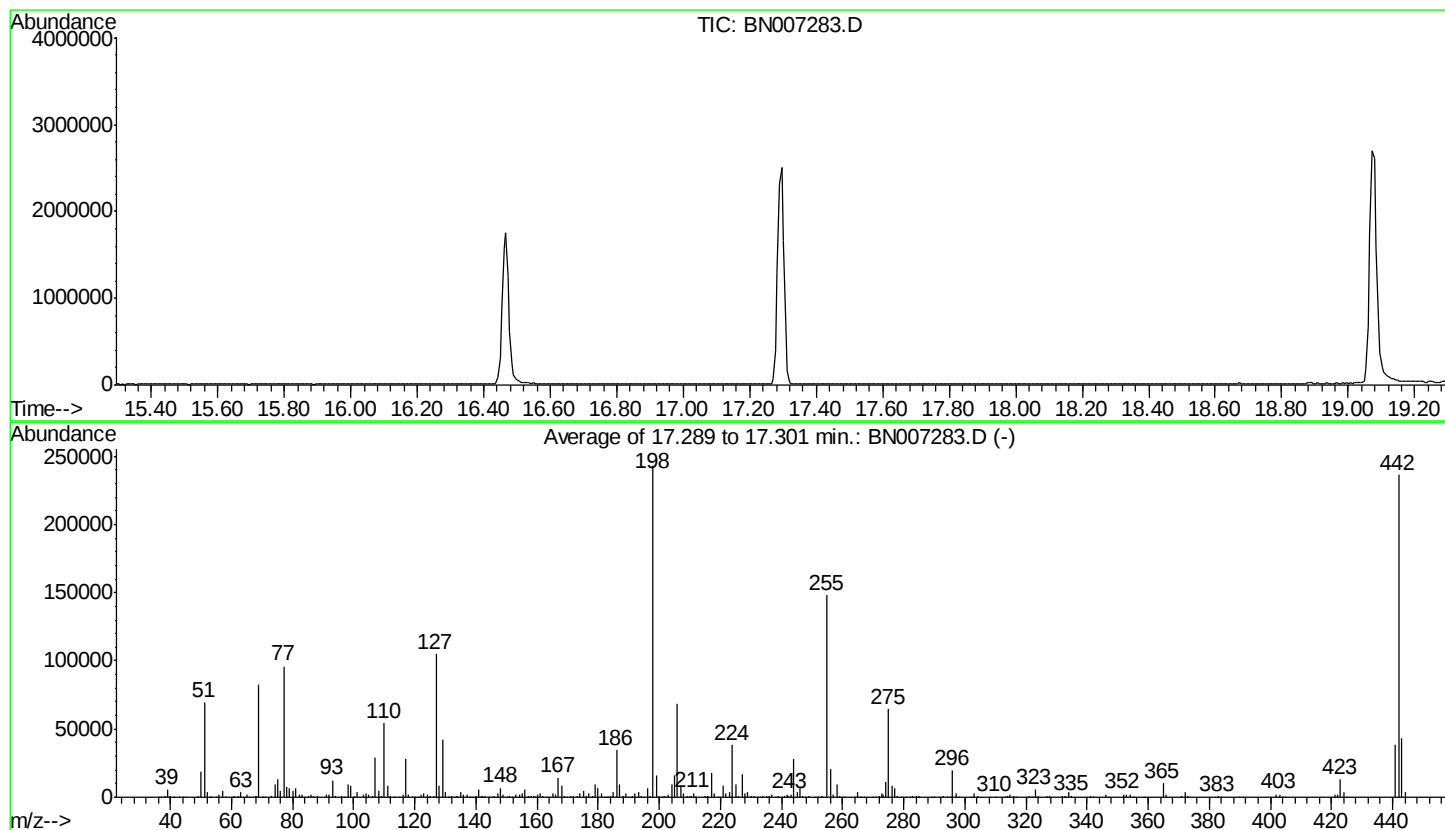

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.4	69130	PASS
68	69	0.00	2	1.1	942	PASS
69	198	0.00	100	33.8	82282	PASS
70	69	0.00	2	0.3	284	PASS
127	198	10	80	43.1	104877	PASS
197	198	0.00	2	0.5	1209	PASS
198	198	100	100	100.0	243114	PASS
199	198	5	9	6.6	16081	PASS
275	198	10	60	26.5	64437	PASS
365	198	1	100	4.2	10109	PASS
441	198	0.01	100	15.9	38560	PASS
442	198	50	100	97.2	236373	PASS
443	442	15	24	18.2	43104	PASS