


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN082119\
 Data File : BN007294.D
 Acq On : 21 Aug 2019 17:34
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN082019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Aug 20 18:52:43 2019

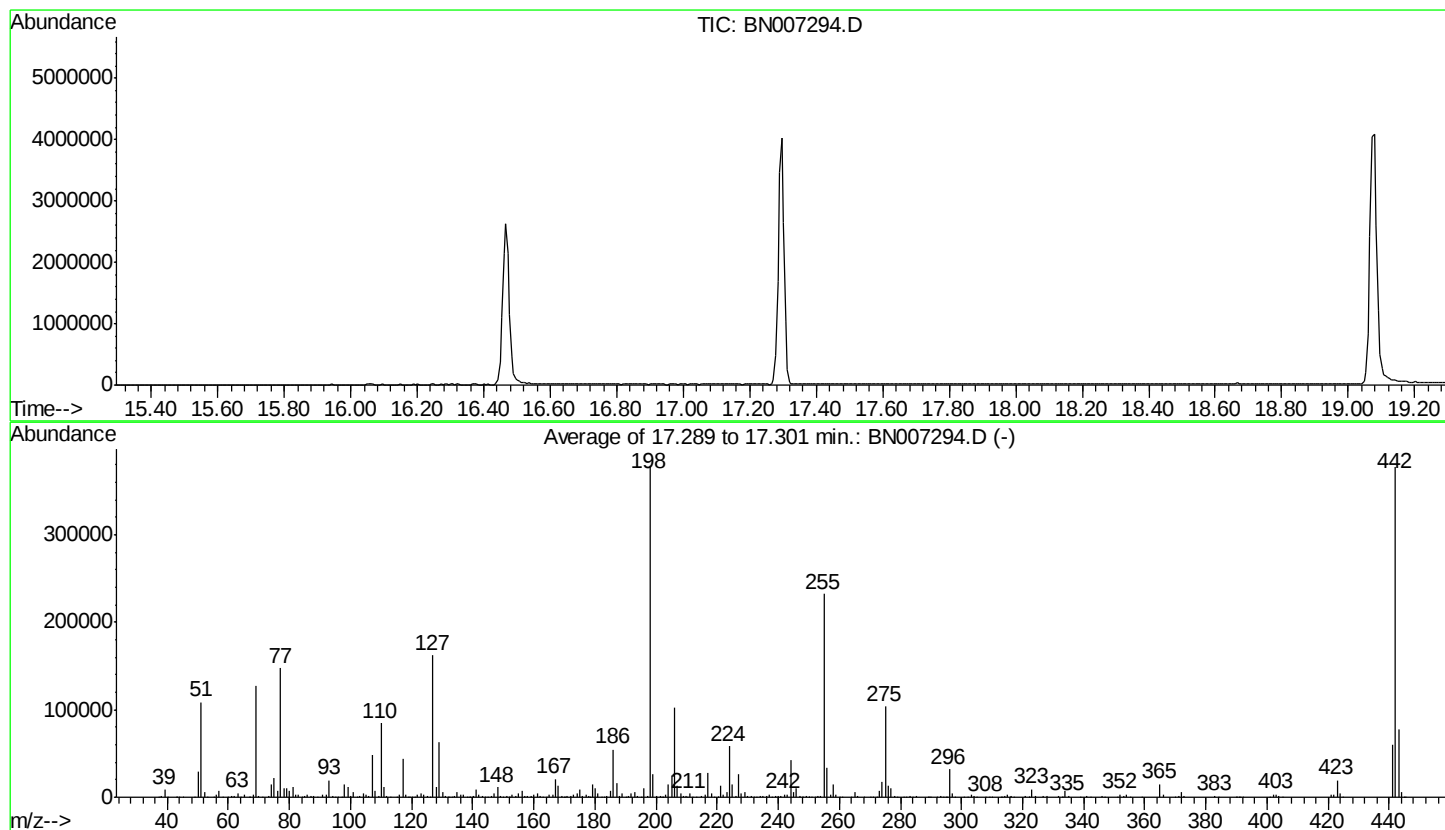

AutoFind: Scans 2457, 2458, 2459; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.7	108750	PASS
68	69	0.00	2	2.0	2539	PASS
69	198	0.00	100	33.6	127520	PASS
70	69	0.00	2	0.7	909	PASS
127	198	10	80	42.7	161933	PASS
197	198	0.00	2	0.3	1262	PASS
198	198	100	100	100.0	379306	PASS
199	198	5	9	6.8	25858	PASS
275	198	10	60	27.4	103848	PASS
365	198	1	100	4.1	15411	PASS
441	198	0.01	100	16.0	60533	PASS
442	198	50	100	99.5	377386	PASS
443	442	15	24	20.6	77722	PASS