

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
 Data File : BN002555.D
 Acq On : 31 Aug 2018 12:14
 Operator : JU/SJ
 Sample : J4665-07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 31 16:12:35 2018
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 04:34:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	173365	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	795341	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	491306	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.04	188	1142311	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	1166528	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1045468	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.23	96	22736	6.19	ng/uL	0.00
5) Phenol-d5	6.85	99	509218	32.04	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	339406	33.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	414568	34.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	431255	33.93	ng/ul	0.00
19) Nitrobenzene-d5	8.81	128	214939	33.95	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	243738	36.61	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	426208	34.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	614486	46.46	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1657238	40.69	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1965569	39.34	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	239253	31.08	ng/ul	0.00
57) Fluorene-d10	15.30	176	1410671	39.95	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	222273	30.56	ng/ul	0.00
70) Anthracene-d10	17.14	188	2234866	40.95	ng/ul	0.00
78) Pyrene-d10	19.44	212	2450292	43.90	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	2284031	41.78	ng/ul	0.00
Target Compounds						
15) N-Nitroso-di-n-propylamine	8.37	70	11407	1.064	ng/ul#	1
44) Dimethylphthalate	13.76	163	470401	11.776	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002555.D
Acq On : 31 Aug 2018 12:14
Operator : JU/SJ
Sample : J4665-07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 31 16:12:35 2018
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 04:34:18 2018
Response via : Initial Calibration

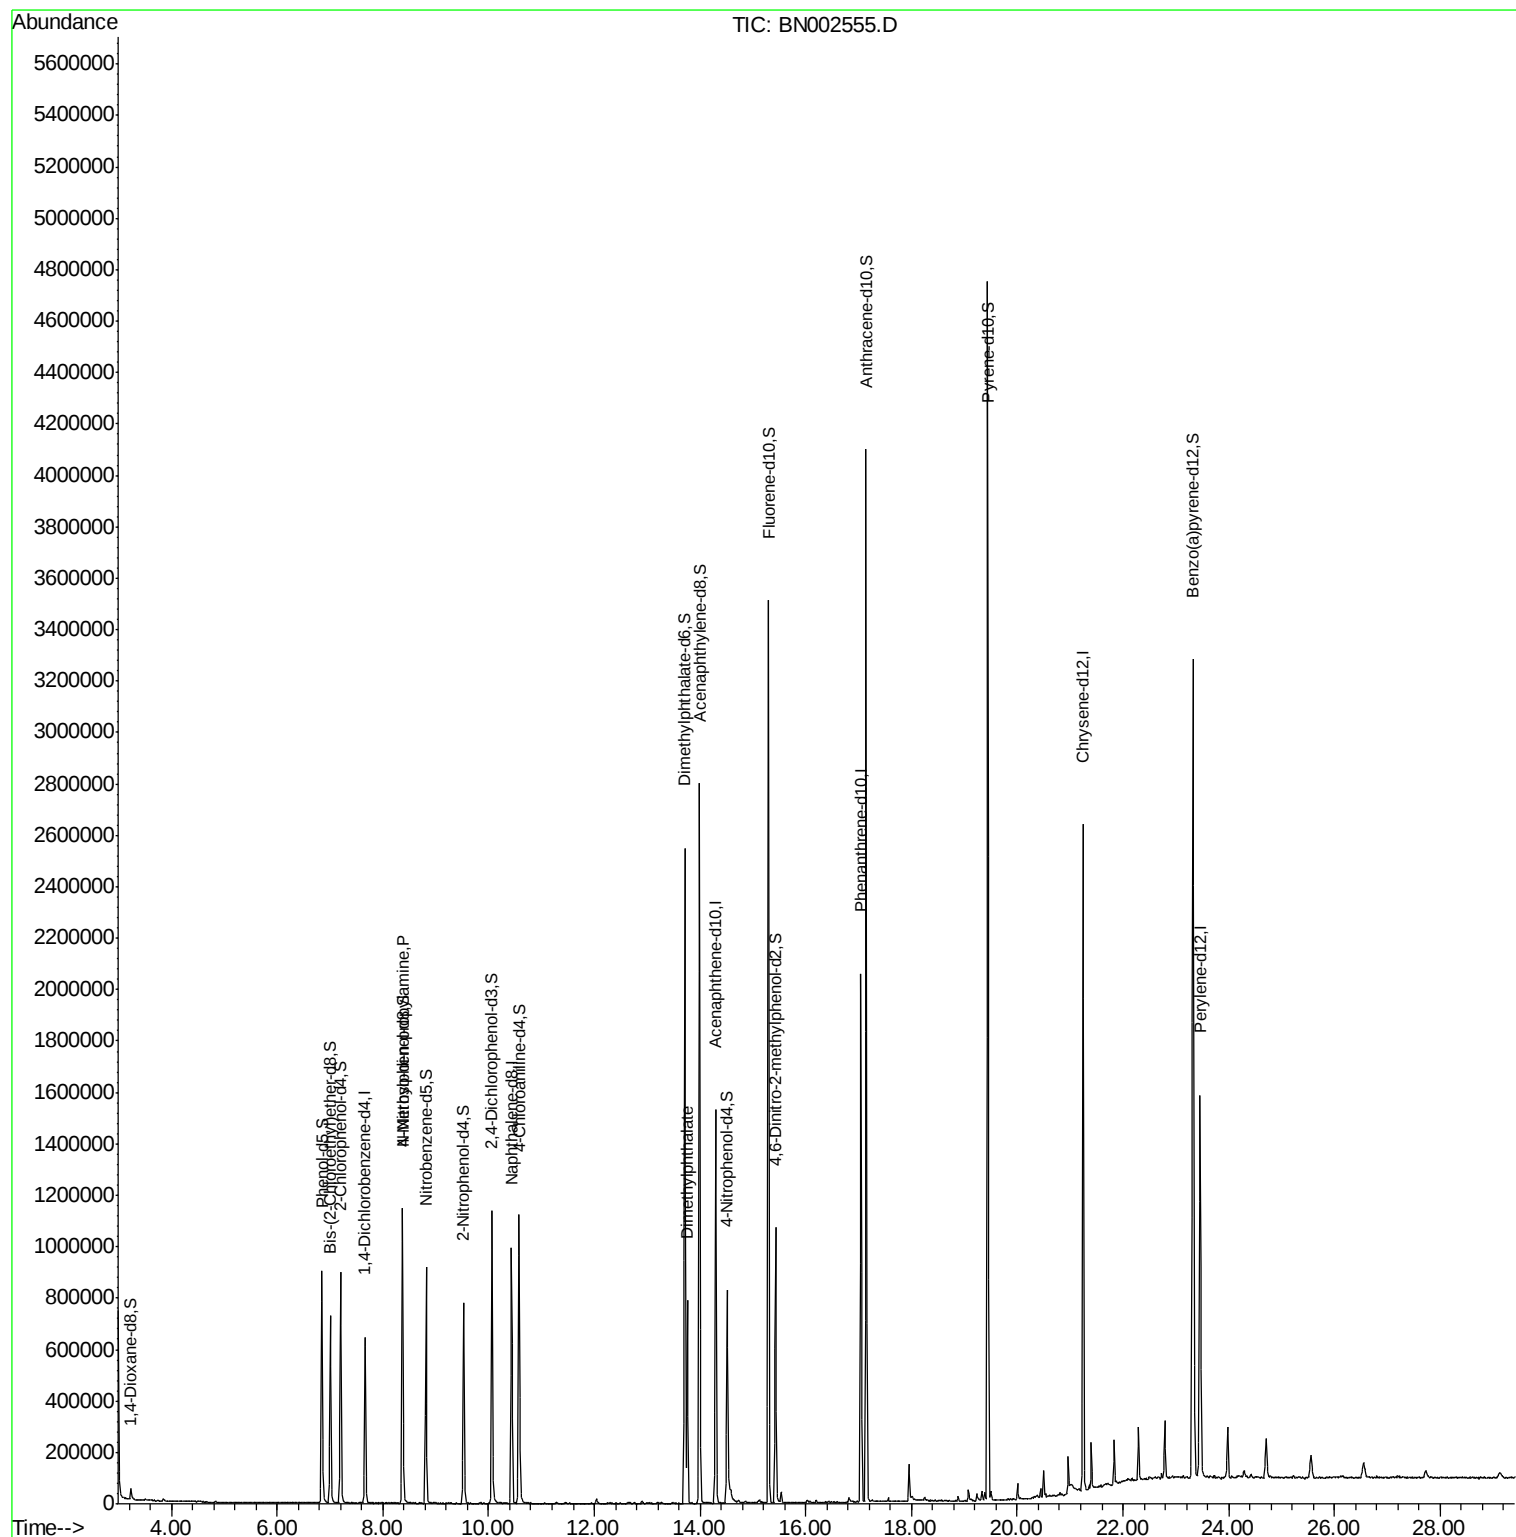

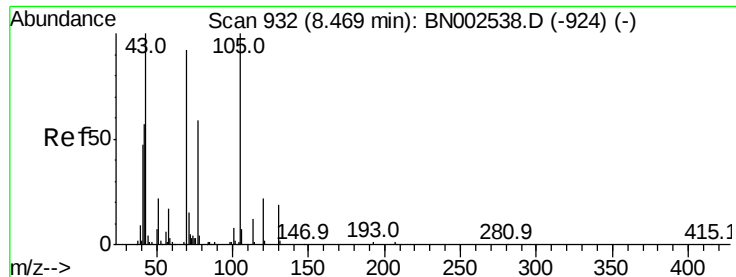

#15

N-Nitroso-di-n-propylamine

Concen: 1.064 ng/ul

RT: 8.37 min Scan# 915

Delta R.T. -0.10 min

Lab File: BN002555.D

Acq: 31 Aug 2018 12:14

Instrument :

BNA_N

ClientSampleId :

Tot Ion: 70 Resp: 11407





Ion Ratio Lower Upper

70 100

42 399.2 35.4 53.0#

101 0.0 8.4 12.6#

130 0.0 18.2 27.4#

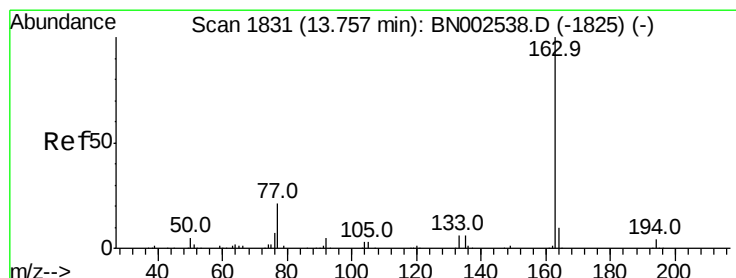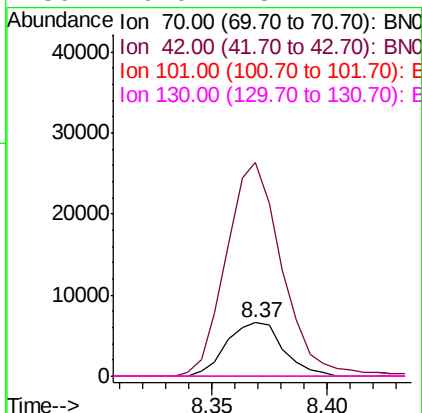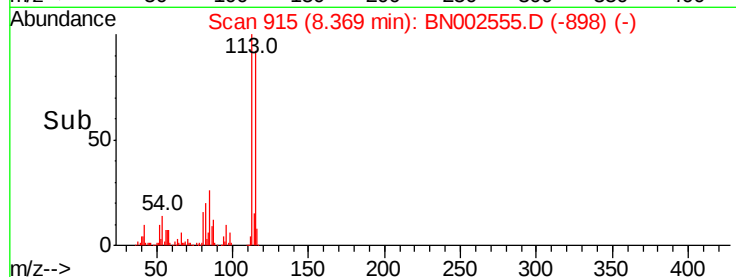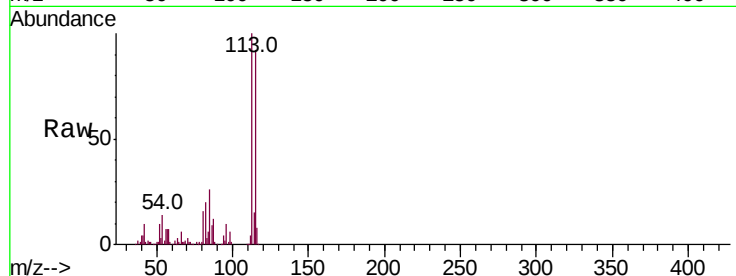

#44

Dimethylphthalate

Concen: 11.776 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN002555.D

Acq: 31 Aug 2018 12:14

Tgt Ion:163 Resp: 470401

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 9.9 7.8 11.8

