

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
 Data File : BN002564.D
 Acq On : 31 Aug 2018 17:29
 Operator : JU/SJ
 Sample : J4665-06
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Aug 31 23:10:09 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 31 23:07:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	156064	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	734486	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	453388	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1063052	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1157139	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1118900	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	19470	5.89	ng/uL	0.00
5) Phenol-d5	6.85	99	426441	29.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.01	67	287745	32.01	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	353326	32.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	366604	32.05	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	185208	31.68	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	213630	34.74	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	376993	33.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	557413	45.64	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1422449	37.85	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1702819	36.93	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	187879	26.44	ng/ul	0.00
57) Fluorene-d10	15.29	176	1215302	37.30	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	191481	28.29	ng/ul	0.00
70) Anthracene-d10	17.15	188	1921676	37.84	ng/ul	0.00
78) Pyrene-d10	19.45	212	2173063	39.25	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	2312629	39.53	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.76	163	509004	13.809	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002564.D
Acq On : 31 Aug 2018 17:29
Operator : JU/SJ
Sample : J4665-06
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :

Quant Time: Aug 31 23:10:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 31 23:07:10 2018
Response via : Initial Calibration

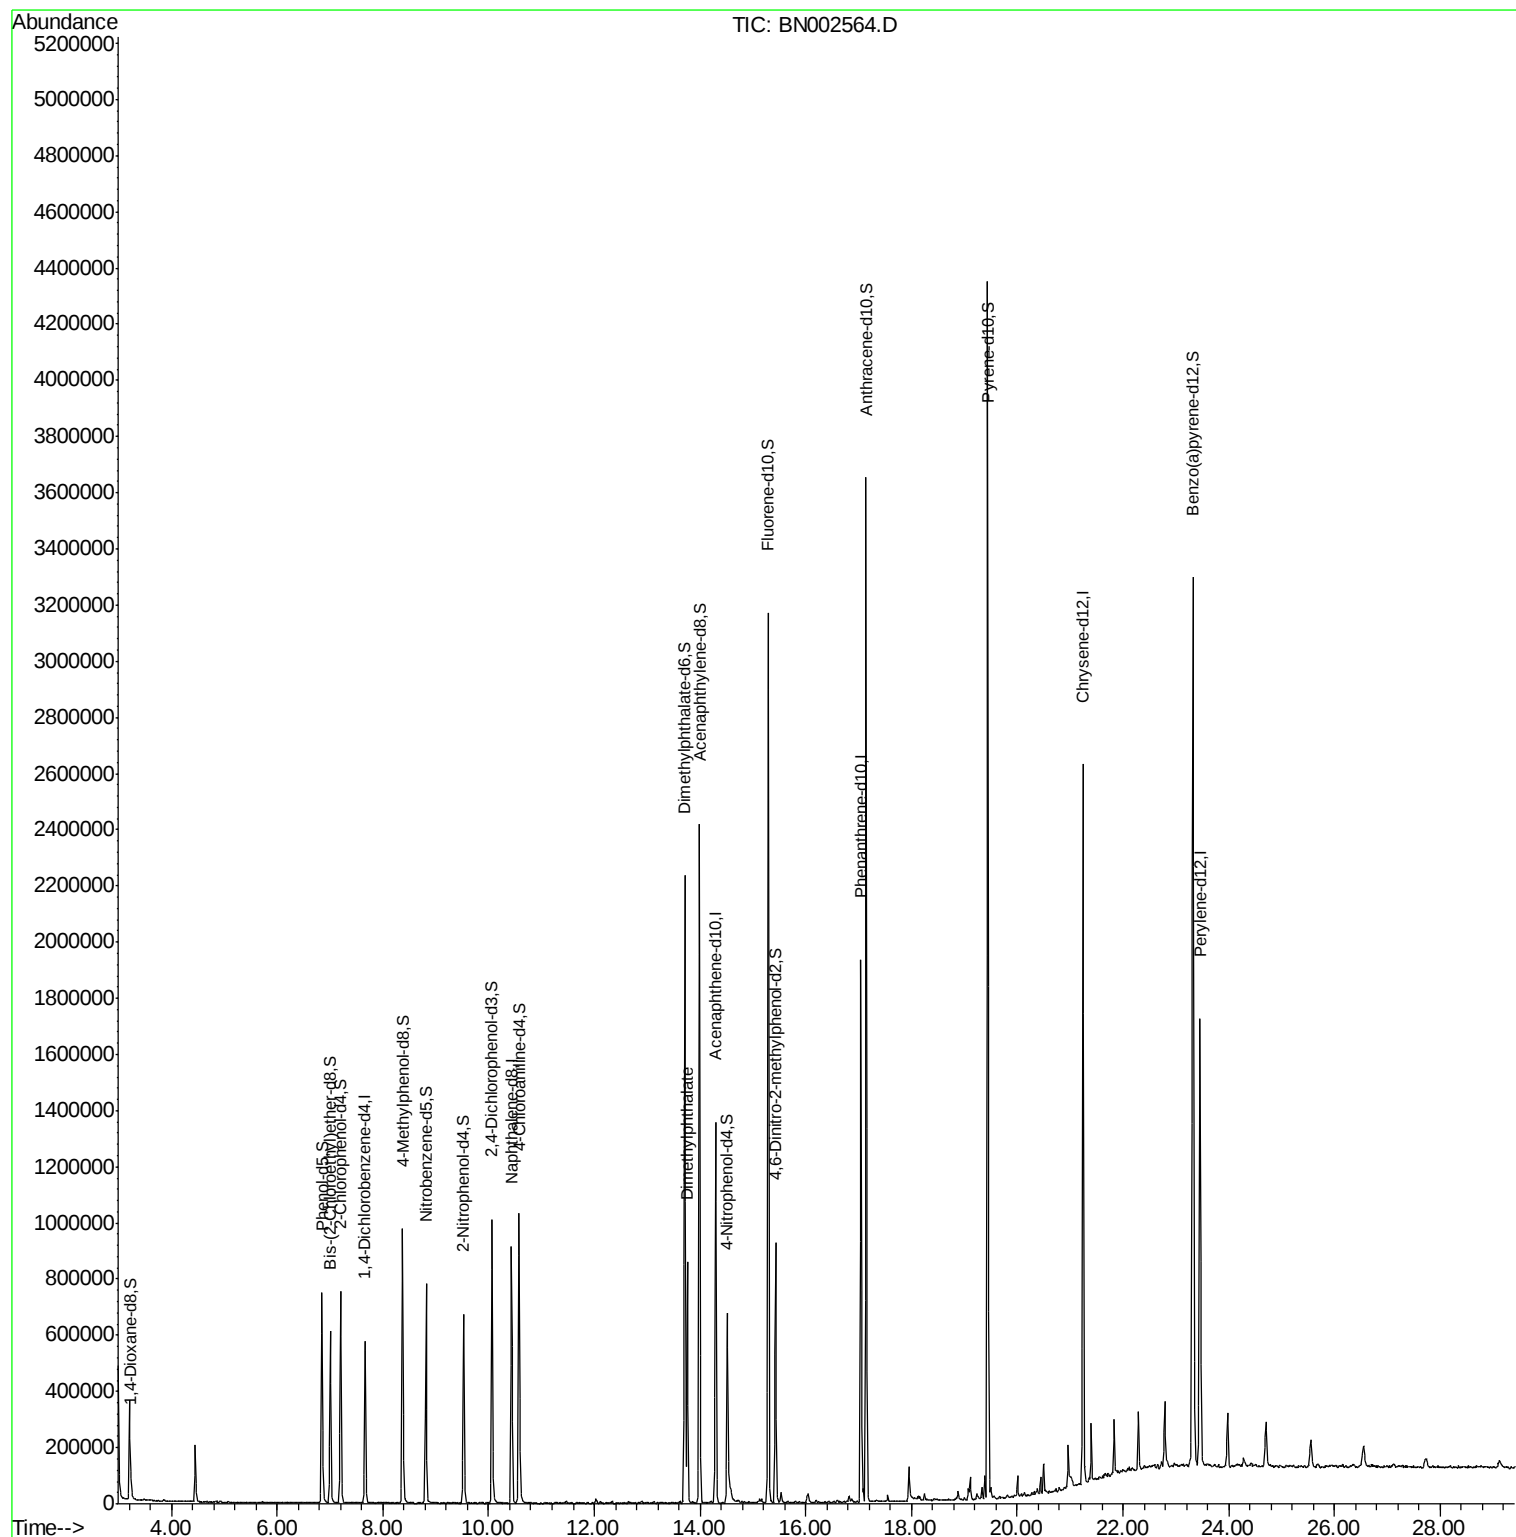


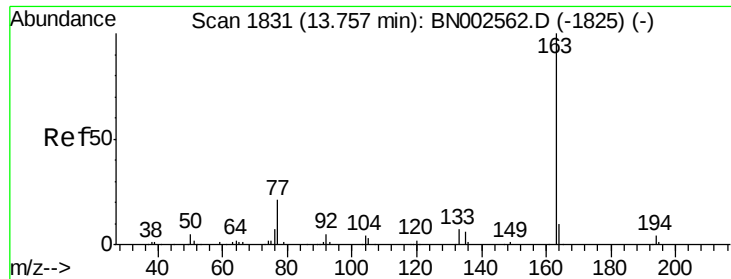

#44
 Dimethylphthalate
 Concen: 13.809 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. 0.00 min
 Lab File: BN002564.D
 Acq: 31 Aug 2018 17:29

Instrument :
 BNA_N
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.2	4.8
164	10.5	7.8	11.8

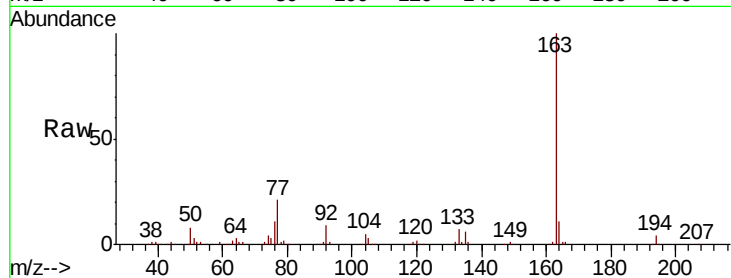

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

