

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
 Data File : BN002559.D
 Acq On : 31 Aug 2018 14:34
 Operator : JU/SJ
 Sample : J4665-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA0

Quant Time: Aug 31 16:12:55 2018
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Aug 25 04:34:18 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	164298	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	772258	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	481660	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1110493	20.00	ng/ul	0.00
77) Chrysene-d12	21.24	240	1167486	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1098622	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	13374	3.84	ng/uL	0.00
5) Phenol-d5	6.85	99	370075	24.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	245459	25.94	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	294184	25.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	352686	29.28	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	170210	27.69	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	206270	31.91	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	362406	30.51	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	825488	64.28	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1506181	37.72	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1759402	35.92	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	178334	23.63	ng/ul	0.00
57) Fluorene-d10	15.29	176	1284142	37.09	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	185502	26.24	ng/ul	0.00
70) Anthracene-d10	17.15	188	2032288	38.31	ng/ul	0.00
78) Pyrene-d10	19.45	212	2238534	40.07	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.32	264	2227088	38.77	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.76	163	394066	10.063	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002559.D
Acq On : 31 Aug 2018 14:34
Operator : JU/SJ
Sample : J4665-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA0

Quant Time: Aug 31 16:12:55 2018
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Aug 25 04:34:18 2018
Response via : Initial Calibration

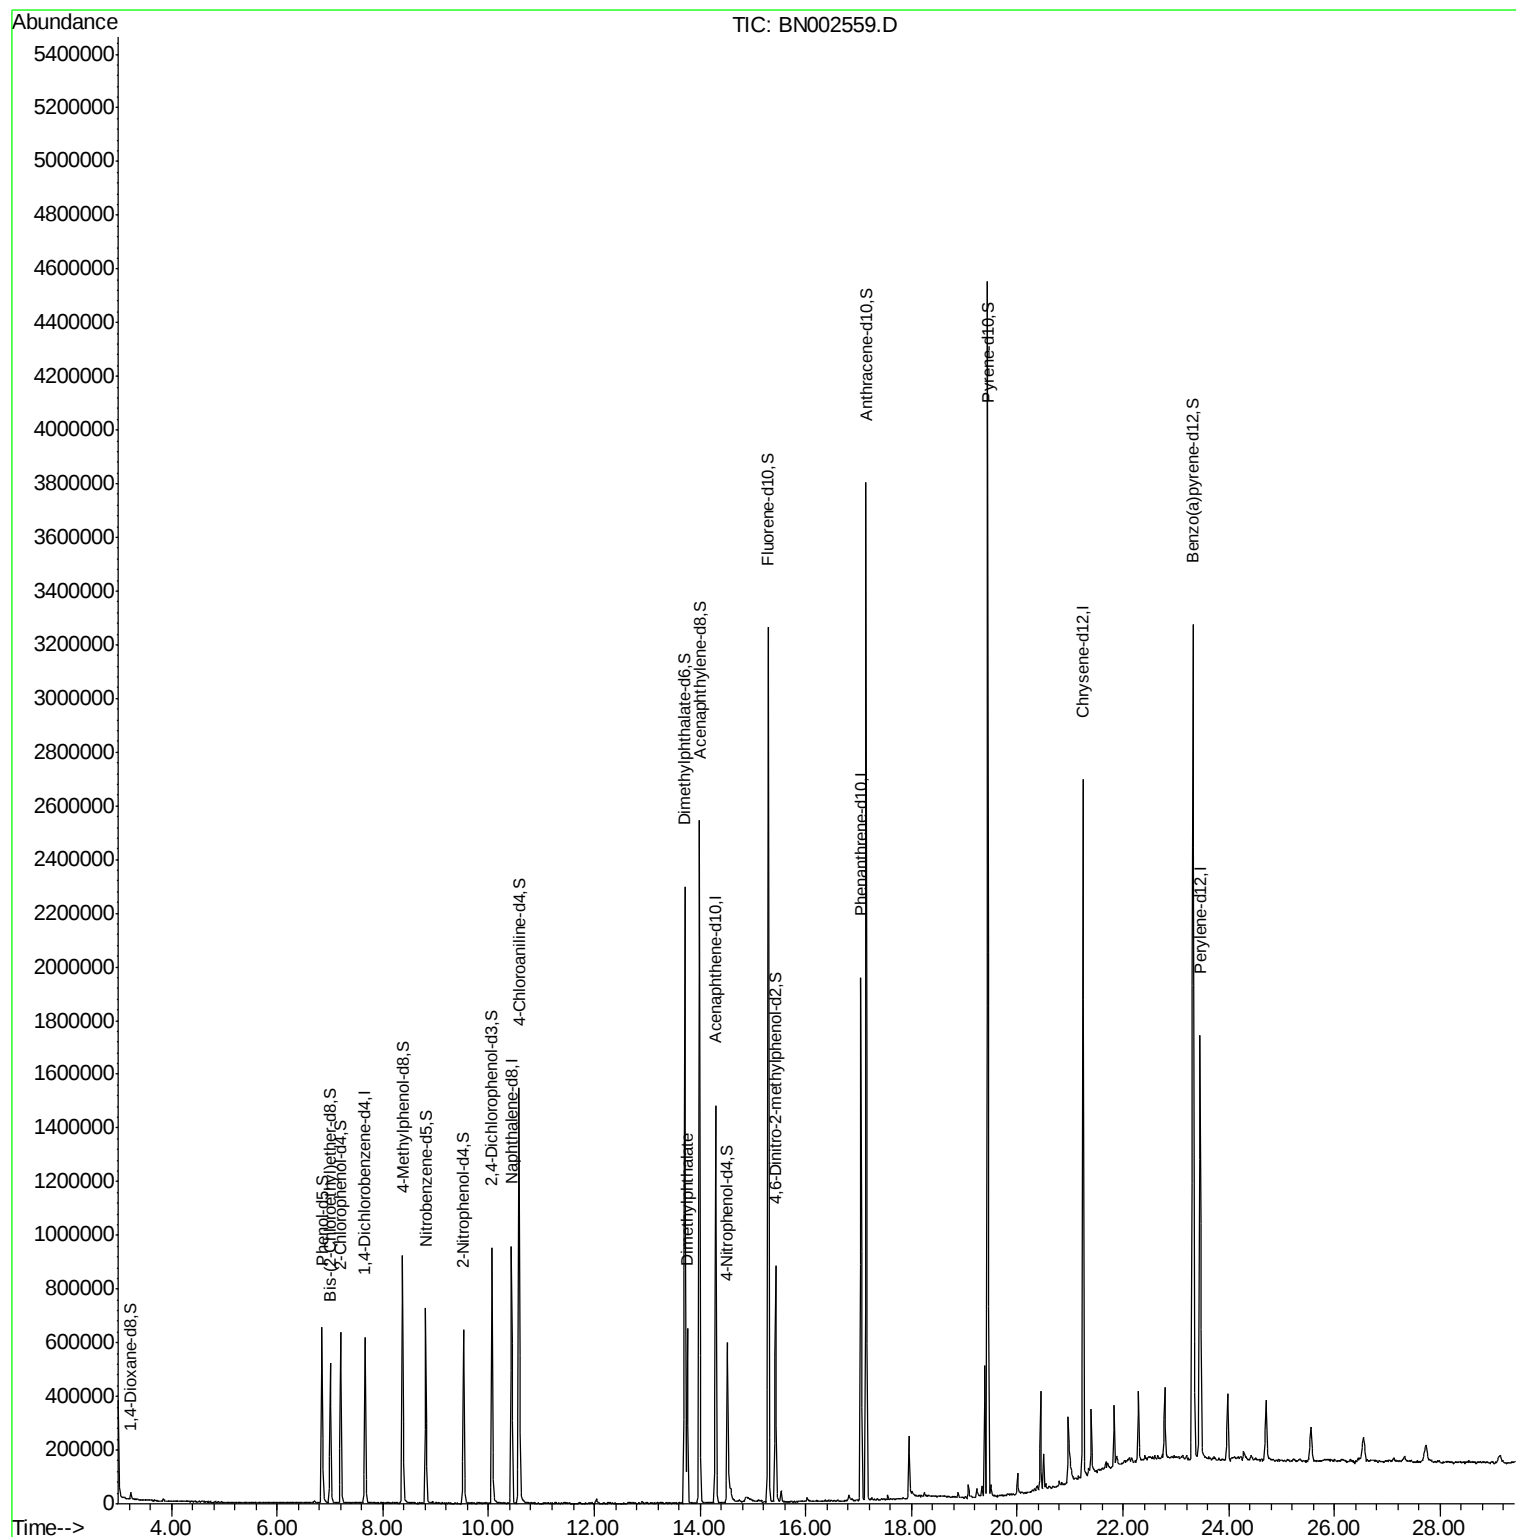

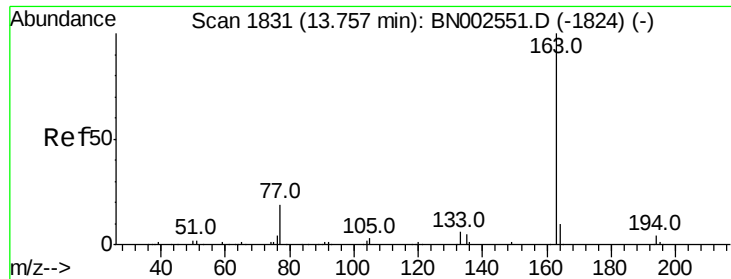

#44

Dimethylphthalate

Concen: 10.063 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. -0.01 min

Lab File: BN002559.D

Acq: 31 Aug 2018 14:34

Instrument :

BNA_N

ClientSampleId :

E0AA0


Tot Ion:163 Resp: 394066

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.5 7.8 11.8

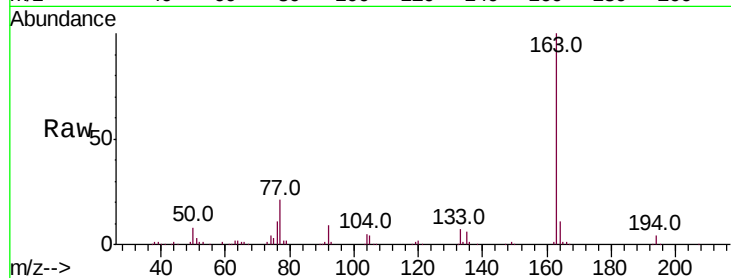

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

