

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN083118\
 Data File : BN002565.D
 Acq On : 31 Aug 2018 18:05
 Operator : JU/SJ
 Sample : J4665-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA1

Quant Time: Aug 31 23:10:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 31 23:07:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	155569	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	730483	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	449163	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	1036754	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1089482	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1033076	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.23	96	15978	4.85	ng/uL	0.00
5) Phenol-d5	6.85	99	386609	27.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	267207	29.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	332631	30.62	ng/ul	0.00
13) 4-Methylphenol-d8	8.37	113	333682	29.26	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	170471	29.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	192639	31.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.06	165	345920	30.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.57	131	486961	40.09	ng/ul	0.00
43) Dimethylphthalate-d6	13.71	166	1222746	32.84	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1560581	34.17	ng/ul	0.00
51) 4-Nitrophenol-d4	14.52	143	168314	23.91	ng/ul	0.00
57) Fluorene-d10	15.29	176	1114906	34.54	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	161637	24.49	ng/ul	0.00
70) Anthracene-d10	17.15	188	1770245	35.74	ng/ul	0.00
78) Pyrene-d10	19.45	212	1915093	36.74	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1933645	35.80	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	13.76	163	372091	10.189	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002565.D
Acq On : 31 Aug 2018 18:05
Operator : JU/SJ
Sample : J4665-04
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA1

Quant Time: Aug 31 23:10:14 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 31 23:07:10 2018
Response via : Initial Calibration

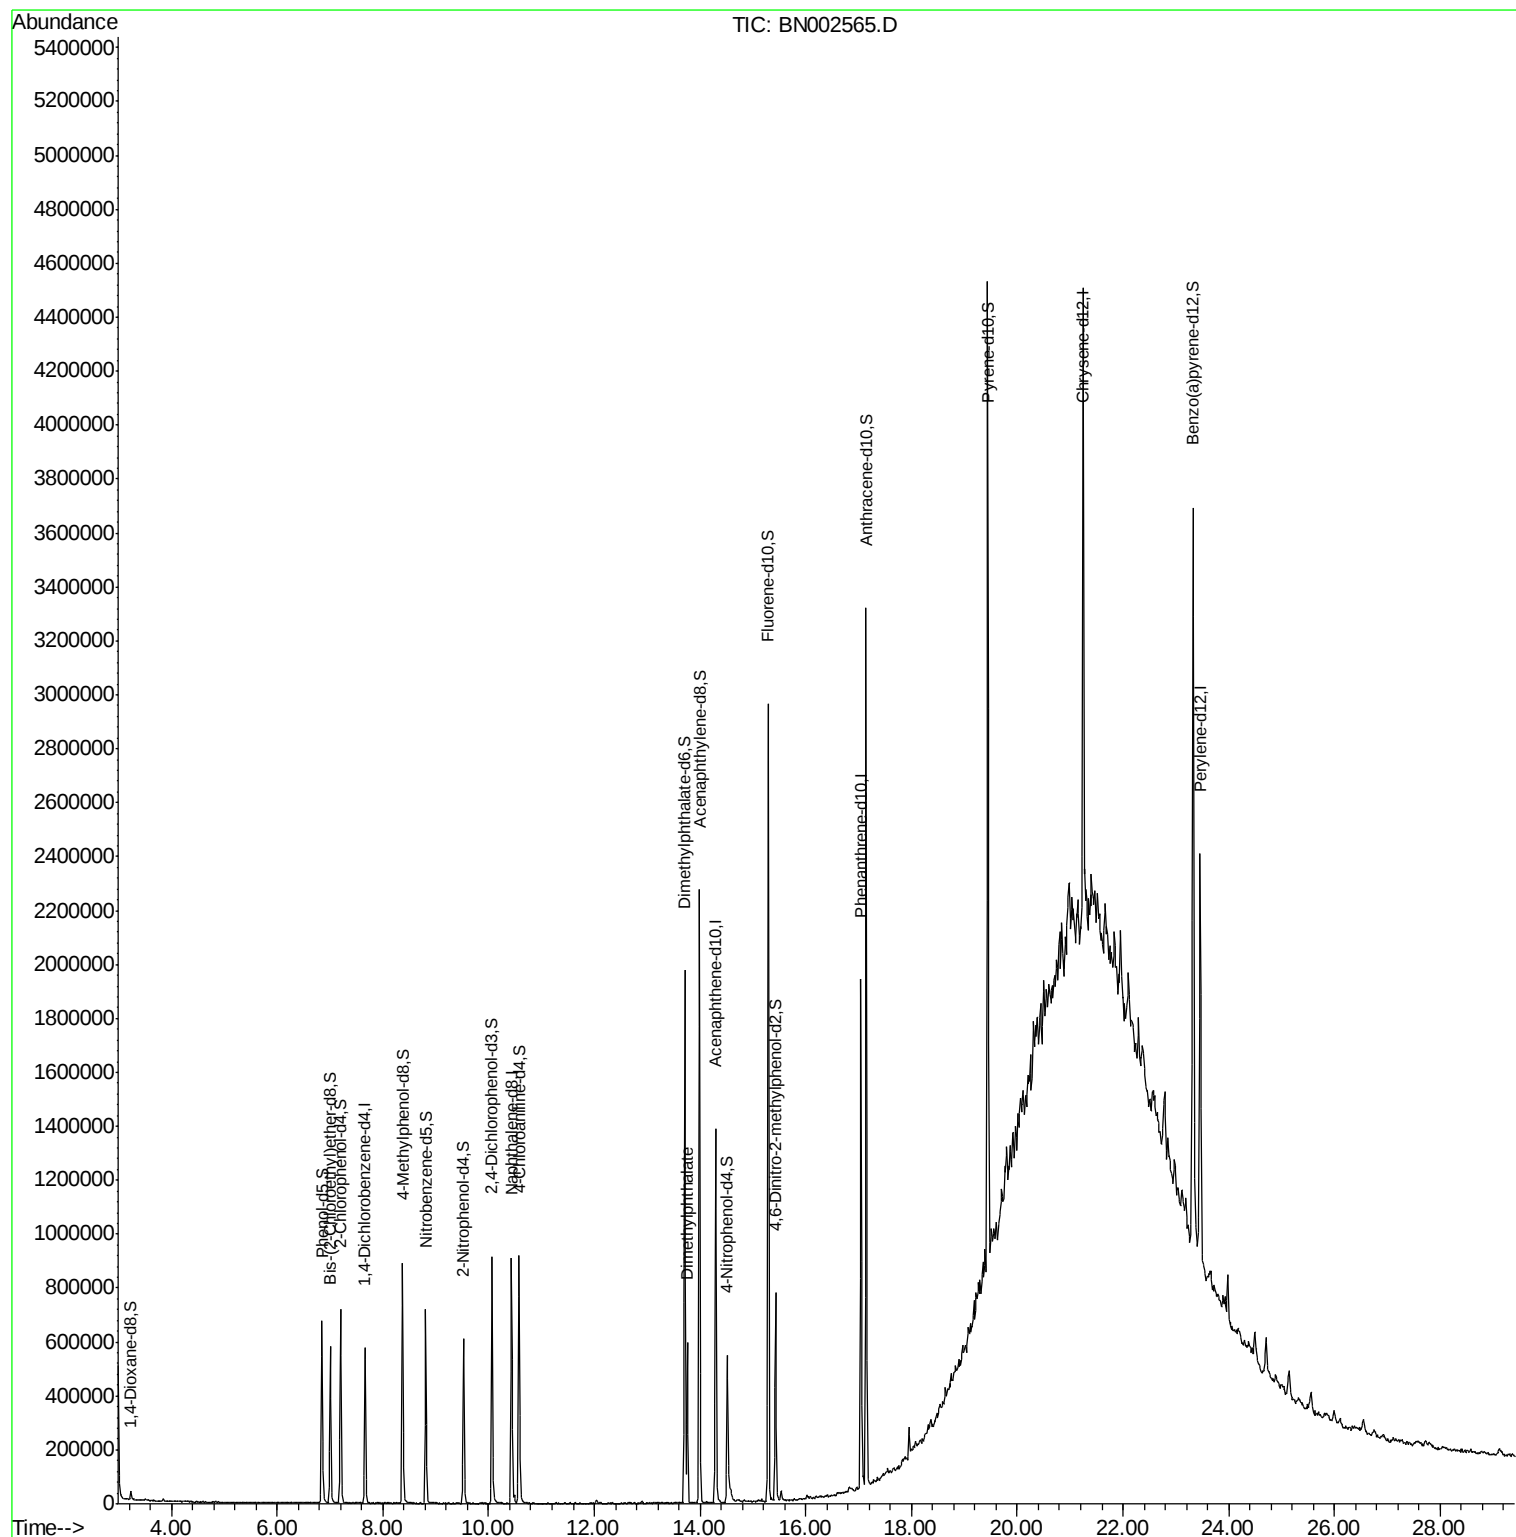

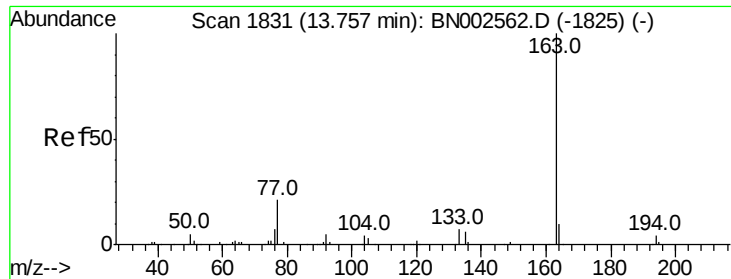

#44

Dimethylphthalate

Concen: 10.189 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. 0.00 min

Lab File: BN002565.D

Acq: 31 Aug 2018 18:05

Instrument :

BNA_N

ClientSampleId :

E0AA1


Tot Ion:163 Resp: 372091

Ion Ratio Lower Upper

163 100

194 4.1 3.2 4.8

164 10.7 7.8 11.8

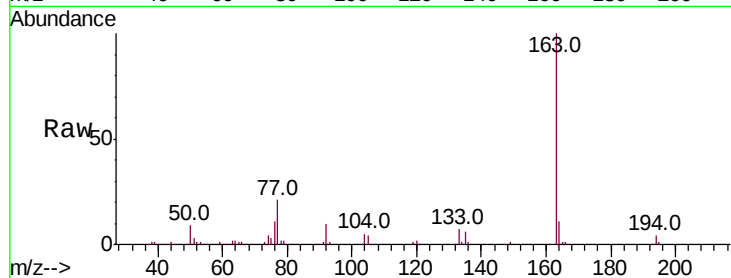

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

