

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
 Data File : BN002572.D
 Acq On : 31 Aug 2018 22:10
 Operator : JU/SJ
 Sample : J4665-15
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AB0

Manual Integrations
 APPROVED

Sohil
 9/4/2018 4:38:12 PM

Quant Time: Aug 31 23:41:00 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 31 23:07:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	155670	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	715644	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	427815	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	976073	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	956742	20.00	ng/ul	0.00
85) Perylene-d12	23.47	264	800323	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	20225	6.13	ng/uL	0.00
5) Phenol-d5	6.85	99	135368	9.48	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	284344	31.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	331132	30.46	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	241565	21.17	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	193699	34.00	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	224662	37.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	392653	35.67	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	20412m	1.72	ng/ul	0.02
43) Dimethylphthalate-d6	13.72	166	1310291	36.95	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1570846	36.11	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	63188	9.43	ng/ul	0.02
57) Fluorene-d10	15.29	176	1107978	36.03	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	219555	35.33	ng/ul	0.00
70) Anthracene-d10	17.15	188	1731110	37.12	ng/ul	0.00
78) Pyrene-d10	19.45	212	1868698	40.82	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1569713	37.51	ng/ul	0.00

Target Compounds					Ovalue
44) Dimethylphthalate	13.76	163	65708	1.889	ng/ul 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002572.D
Acq On : 31 Aug 2018 22:10
Operator : JU/SJ
Sample : J4665-15
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
E0AB0

Quant Time: Aug 31 23:41:00 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 31 23:07:10 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
9/4/2018 4:38:12 PM

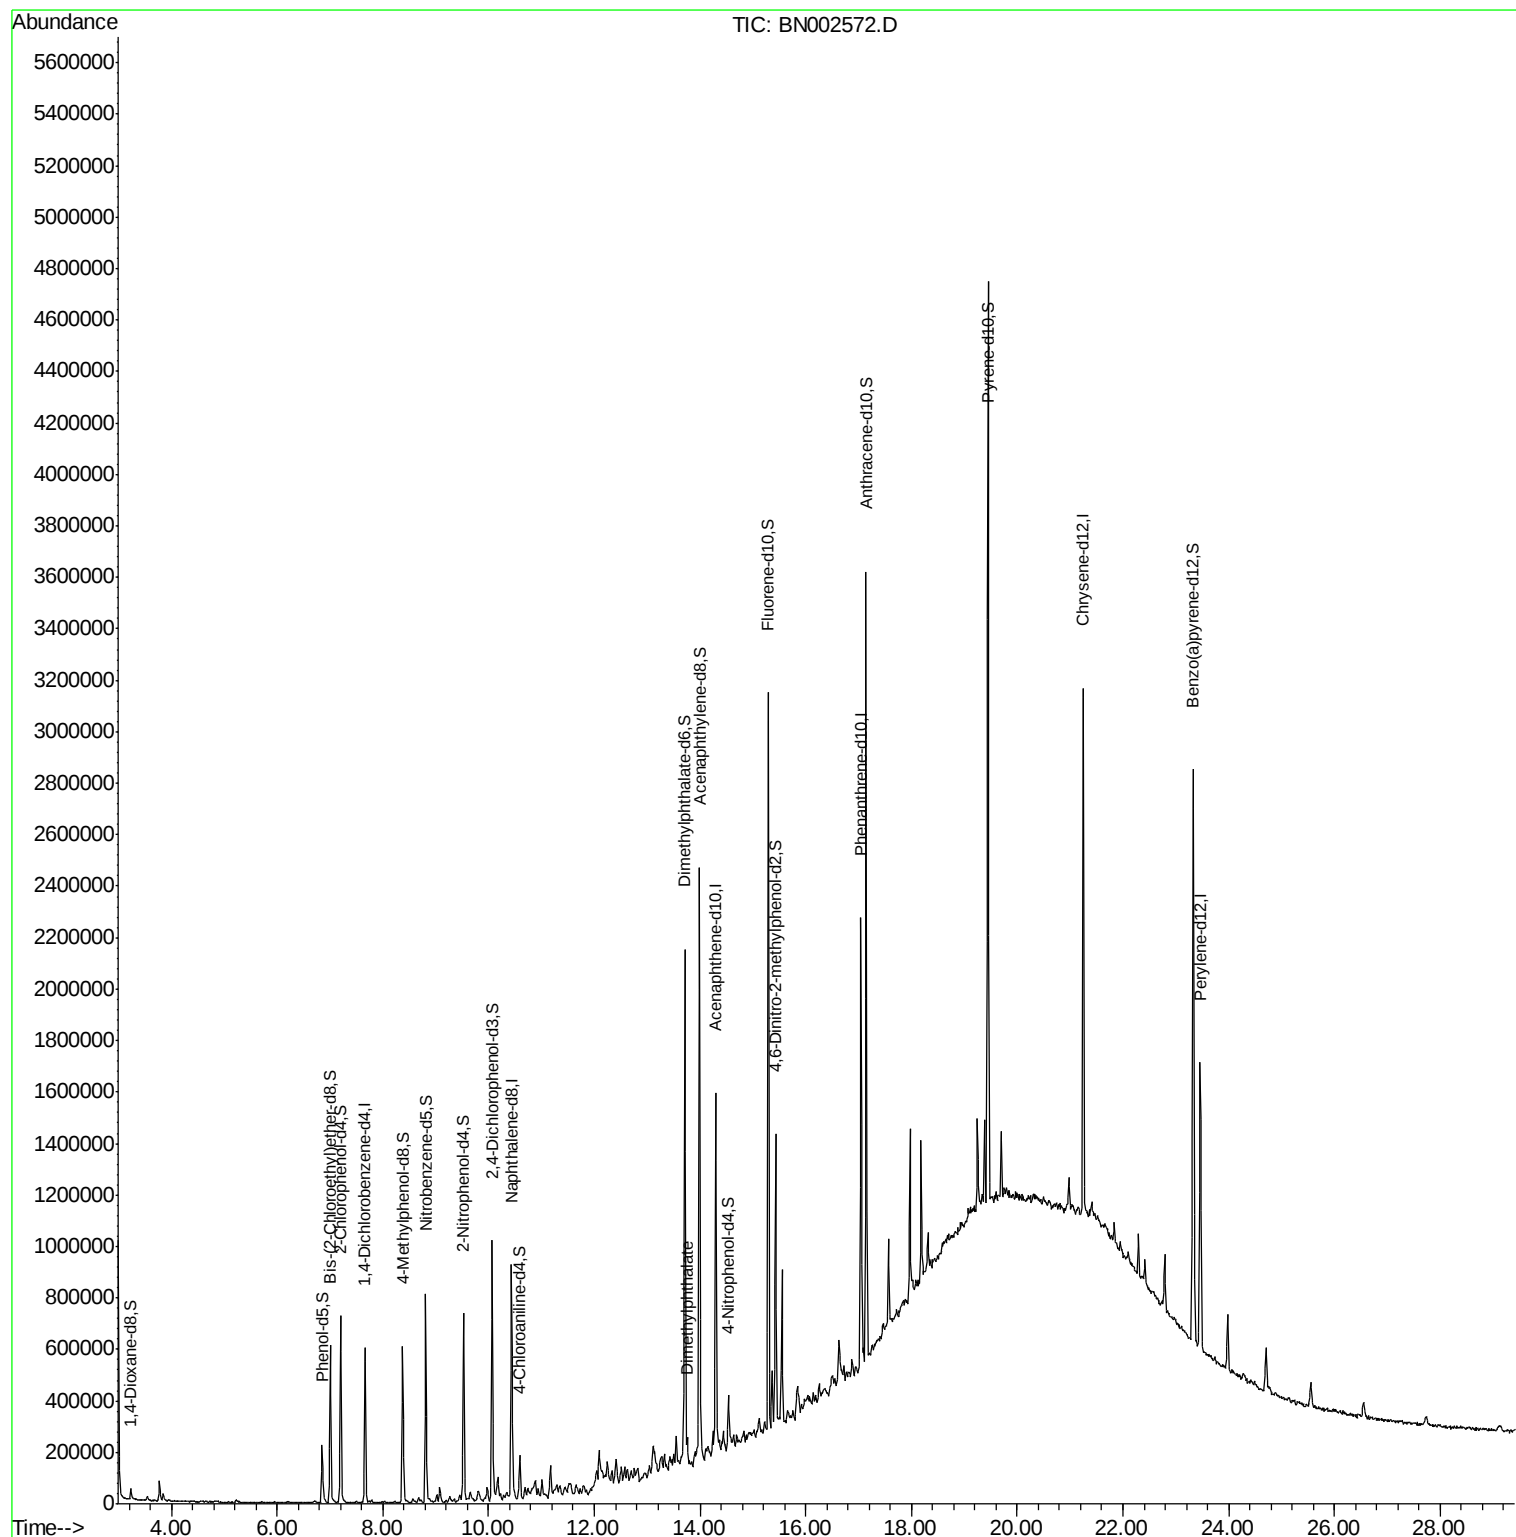

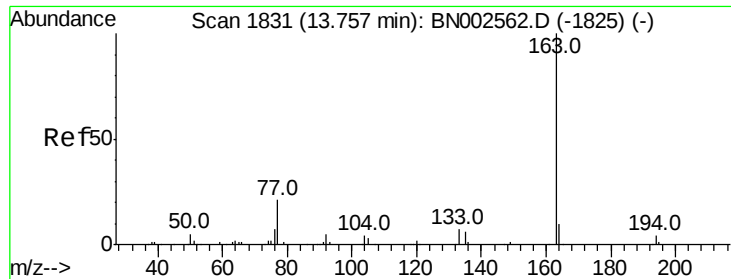

#44
 Dimethylphthalate
 Concen: 1.889 ng/ul
 RT: 13.76 min Scan# 1831
 Delta R.T. 0.00 min
 Lab File: BN002572.D
 Acq: 31 Aug 2018 22:10

Instrument :
 BNA_N
 ClientSampleId :
 E0AB0

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.2	4.8
164	11.2	7.8	11.8

Manual Integrations
 APPROVED

Sohil
 9/4/2018 4:38:12 PM

