

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN083118\
 Data File : BN002573.D
 Acq On : 31 Aug 2018 22:45
 Operator : JU/SJ
 Sample : J4665-12
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AA6

Quant Time: Aug 31 23:55:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Aug 31 23:07:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	159086	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	736783	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.30	164	438697	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.05	188	992938	20.00	ng/ul	0.00
77) Chrysene-d12	21.25	240	1043893	20.00	ng/ul	0.00
85) Perylene-d12	23.46	264	1022951	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.23	96	21375	6.34	ng/uL	0.00
5) Phenol-d5	6.85	99	114110	7.82	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.00	67	256430	27.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.20	132	293281	26.40	ng/ul	0.00
13) 4-Methylphenol-d8	8.38	113	204931	17.57	ng/ul	0.00
19) Nitrobenzene-d5	8.82	128	172250	29.37	ng/ul	0.00
22) 2-Nitrophenol-d4	9.53	143	199435	32.33	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.07	165	348931	30.79	ng/ul	0.00
29) 4-Chloroaniline-d4	10.59	131	70702	5.77	ng/ul	0.01
43) Dimethylphthalate-d6	13.71	166	1188338	32.68	ng/ul	0.00
46) Acenaphthylene-d8	13.99	160	1408357	31.57	ng/ul	0.00
51) 4-Nitrophenol-d4	14.54	143	45308	6.59	ng/ul	0.02
57) Fluorene-d10	15.29	176	1000459	31.73	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.43	200	193332	30.58	ng/ul	0.00
70) Anthracene-d10	17.15	188	1564960	32.99	ng/ul	0.00
78) Pyrene-d10	19.45	212	1753267	35.10	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.33	264	1805111	33.75	ng/ul	0.00


Target Compounds					Ovalue	
44) Dimethylphthalate	13.76	163	156781	4.396	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002573.D
Acq On : 31 Aug 2018 22:45
Operator : JU/SJ
Sample : J4665-12
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AA6

Quant Time: Aug 31 23:55:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Aug 31 23:07:10 2018
Response via : Initial Calibration

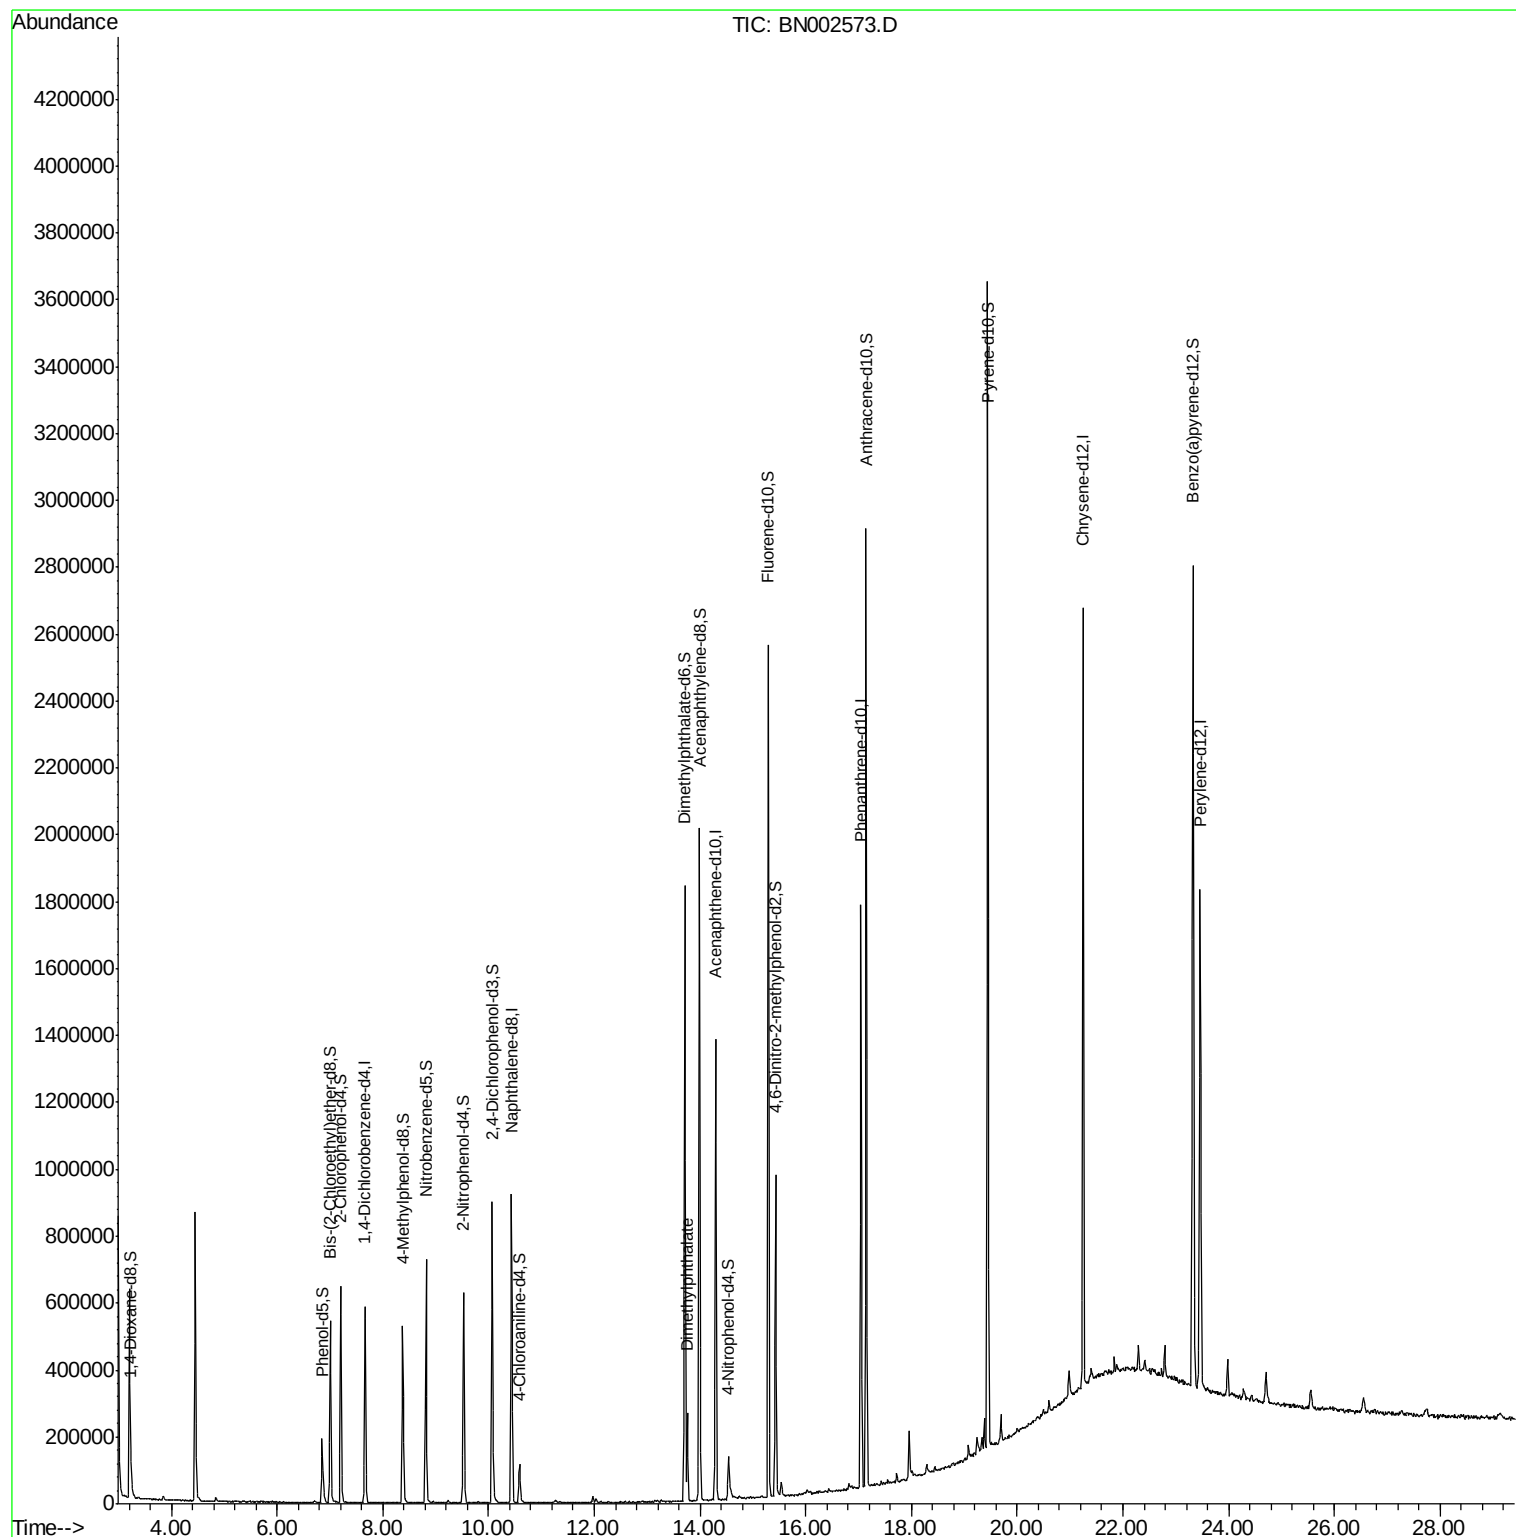

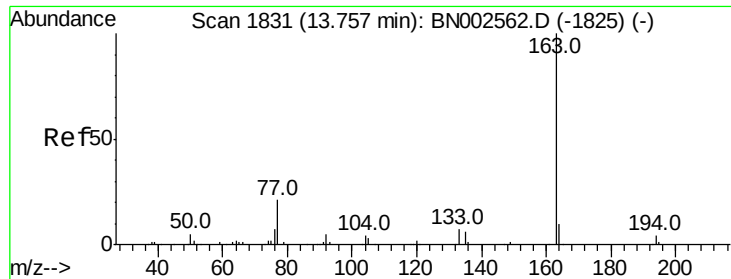

#44

Dimethylphthalate

Concen: 4.396 ng/ul

RT: 13.76 min Scan# 1831

Delta R.T. 0.00 min

Lab File: BN002573.D

Acq: 31 Aug 2018 22:45

Instrument :

BNA_N

ClientSampleId :

E0AA6


Tot Ion:163 Resp: 156781

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.1 7.8 11.8

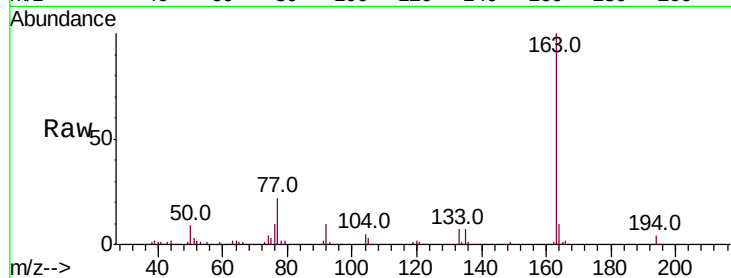

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

