

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
 Data File : BN002569.D
 Acq On : 31 Aug 2018 20:25
 Operator : JU/SJ
 Sample : J4665-17
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E0AB3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SOM-EPA-BN081318MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	6.852	651	657	668	rBV	160681	284888	5.04%	0.608%
2	7.005	677	683	696	rBV	526622	862319	15.25%	1.839%
3	7.205	710	717	731	rVB	586994	961419	17.00%	2.051%
4	7.663	788	795	809	rBV	480667	799159	14.13%	1.705%
5	8.375	910	916	926	rBV	466315	807493	14.28%	1.723%
6	8.816	984	991	1006	rBV	716432	1234185	21.82%	2.633%
7	9.528	1105	1112	1120	rBV	626636	1054752	18.65%	2.250%
8	10.069	1197	1204	1225	rBV	772216	1505874	26.63%	3.212%
9	10.434	1258	1266	1275	rBV	772297	1281464	22.66%	2.734%
10	13.710	1816	1823	1833	rBV	1890247	2708257	47.89%	5.777%
11	13.987	1863	1870	1883	rBV	2167532	3180279	56.24%	6.784%
12	14.298	1916	1923	1938	rVB2	1224009	1885182	33.34%	4.021%
13	14.534	1957	1963	1977	rBV2	97456	246128	4.35%	0.525%
14	15.292	2086	2092	2104	rBV	2743011	4045729	71.54%	8.630%
15	15.428	2109	2115	2129	rVV	986924	1416674	25.05%	3.022%
16	17.045	2384	2390	2399	rVB	1670022	2373501	41.97%	5.063%
17	17.145	2400	2407	2423	rVV2	3191271	4555960	80.56%	9.719%
18	19.445	2792	2798	2806	rBV	3934243	5392648	95.36%	11.503%
19	21.245	3098	3104	3113	rBV2	2275890	2974415	52.60%	6.345%
20	22.292	3278	3282	3289	rBV	96352	131479	2.32%	0.280%
21	22.792	3363	3367	3372	rBV	131887	186041	3.29%	0.397%
22	23.321	3450	3457	3468	rVB	3005610	5655202	100.00%	12.064%
23	23.463	3474	3481	3490	rVB	1481058	2779904	49.16%	5.930%
24	23.980	3564	3569	3576	rVB	151649	284182	5.03%	0.606%
25	24.704	3688	3692	3700	rVB	132058	271303	4.80%	0.579%


Sum of corrected areas: 46878437

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN083118\
Data File : BN002569.D
Acq On : 31 Aug 2018 20:25
Operator : JU/SJ
Sample : J4665-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AB3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

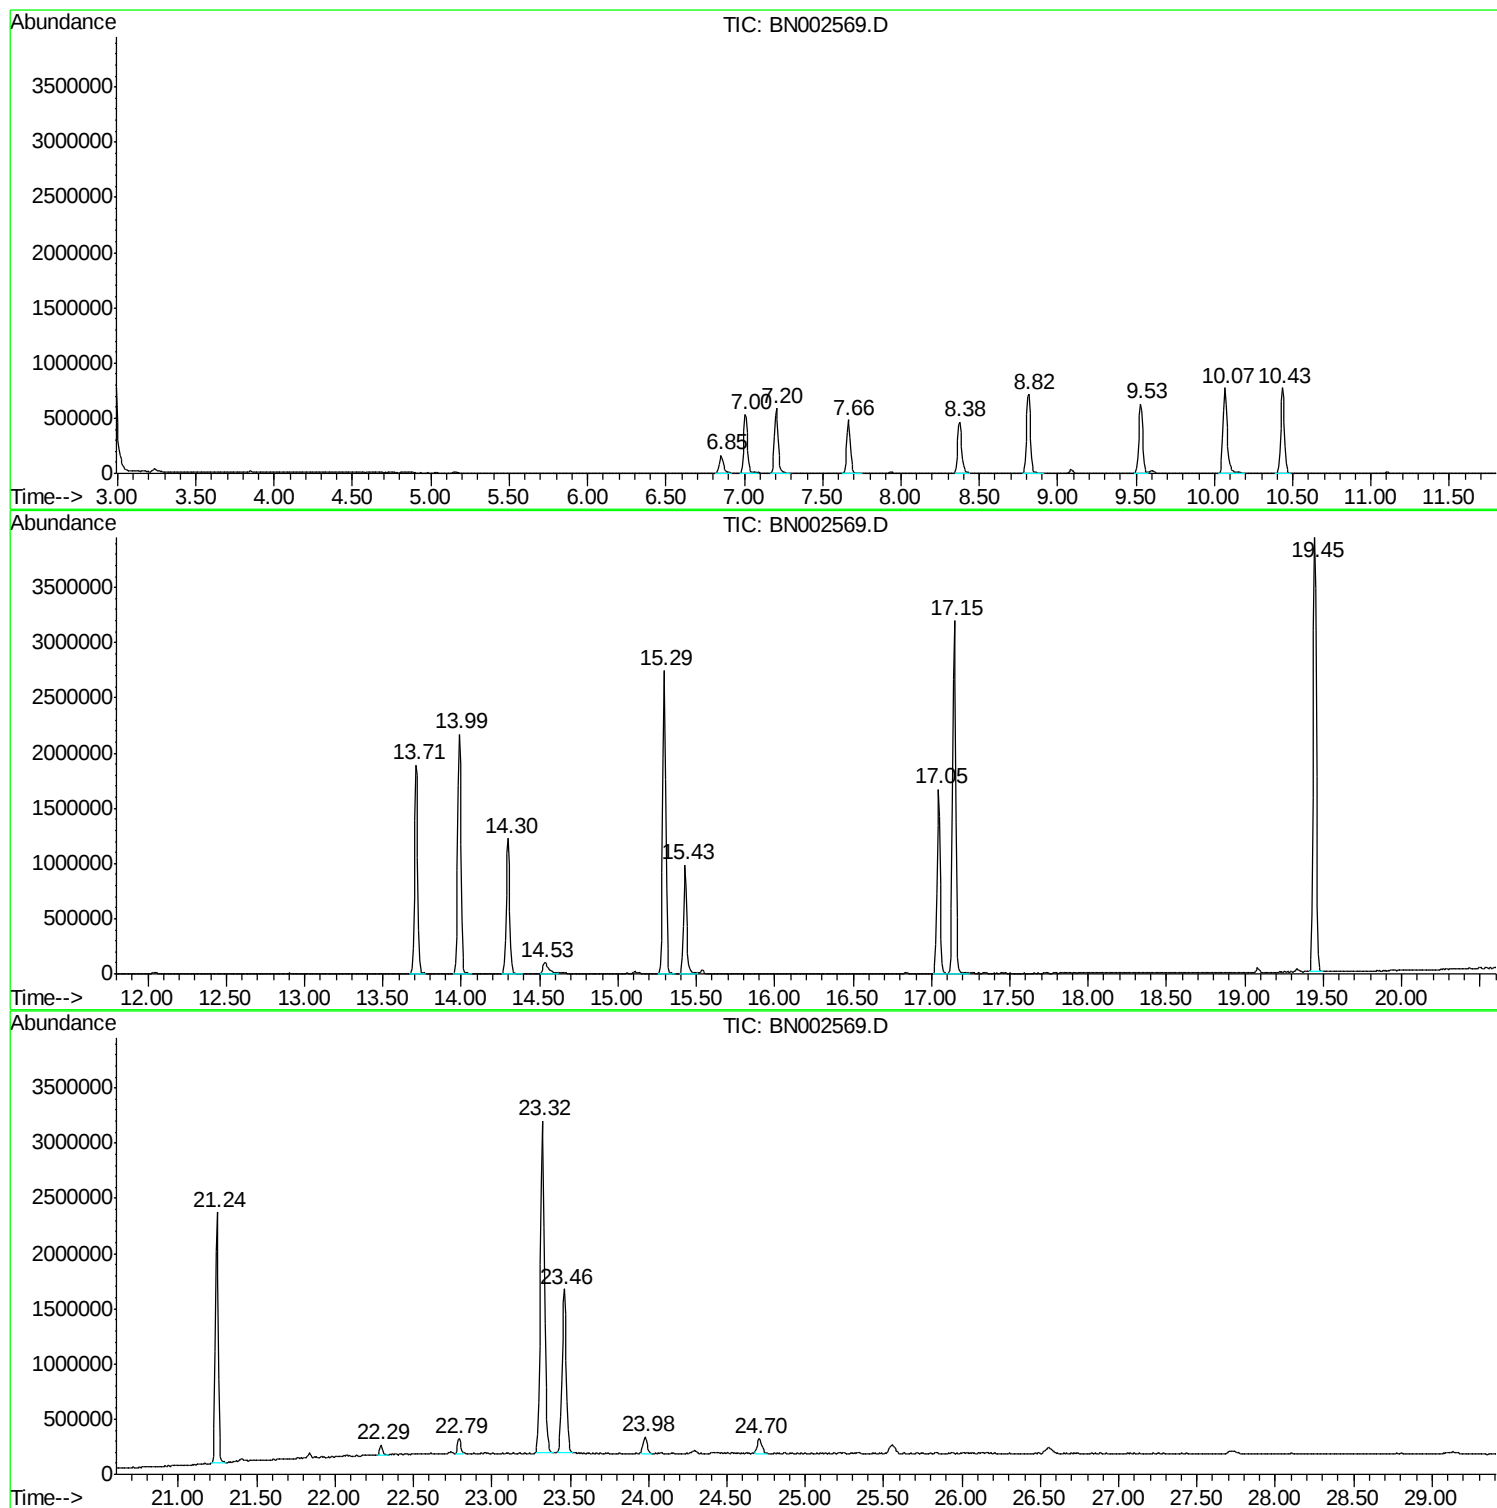

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN083118\
Data File : BN002569.D
Acq On : 31 Aug 2018 20:25
Operator : JU/SJ
Sample : J4665-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AB3










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
23.98	2.04 ng/ul	284182	Perylene-d12	23.46

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Hexacosane			366	C26H54	000630-01-3	90
2	Pentacosane			352	C25H52	000629-99-2	90
3	Hexacosane			366	C26H54	000630-01-3	90
4	Tetracosane			338	C24H50	000646-31-1	90
5	Heneicosane			296	C21H44	000629-94-7	90

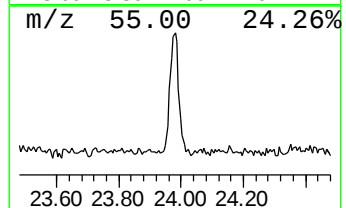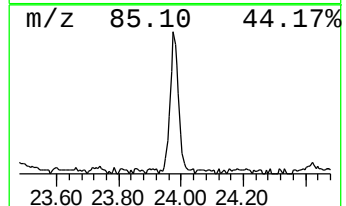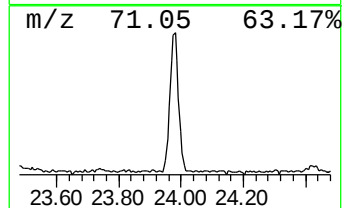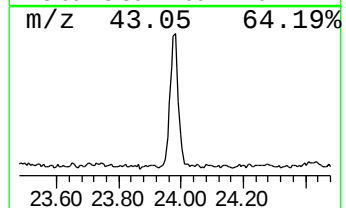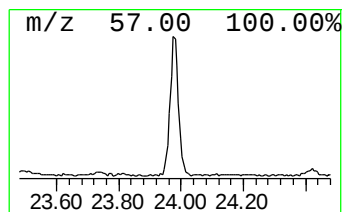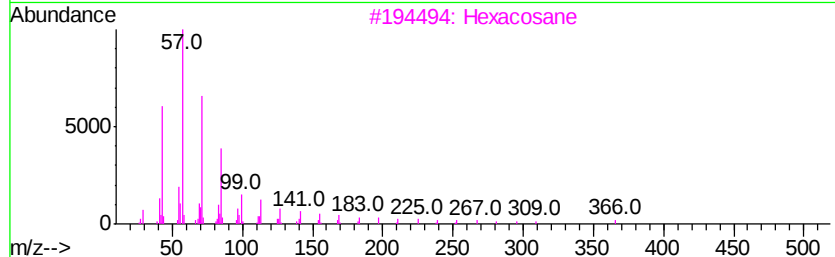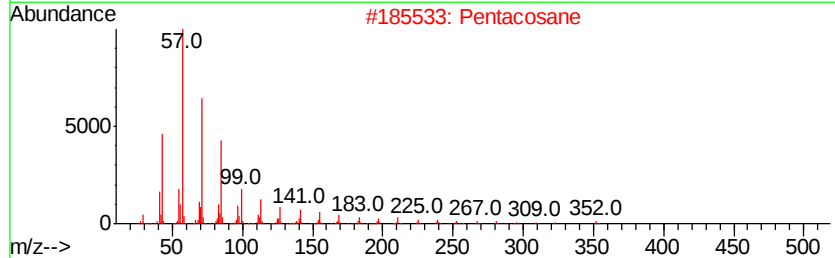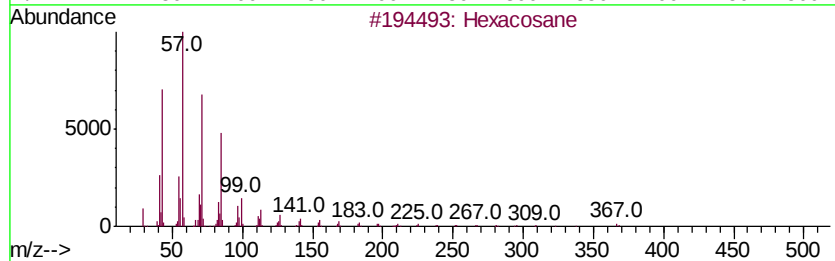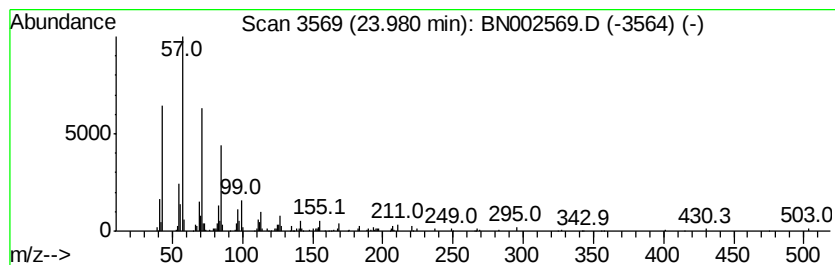

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN083118\
Data File : BN002569.D
Acq On : 31 Aug 2018 20:25
Operator : JU/SJ
Sample : J4665-17
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E0AB3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-BN081318MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: Str...	23.98	2.0	ng/ul	284182	6	23.46	2779900	20.0