
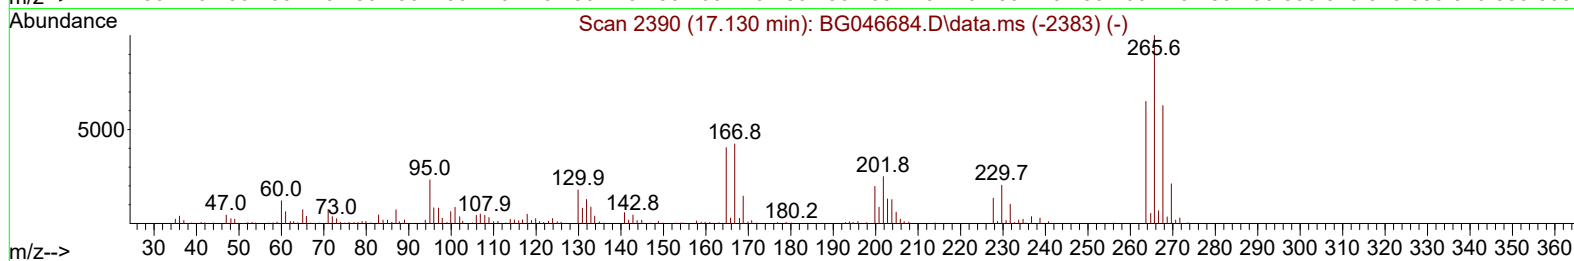
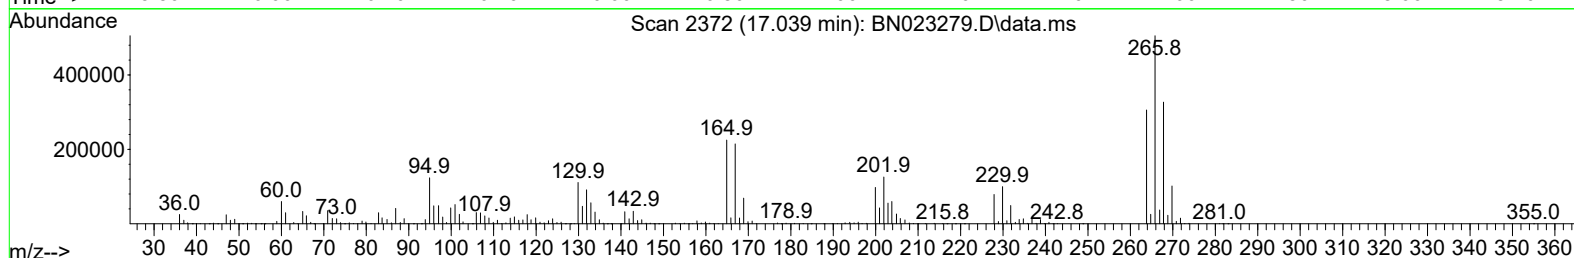


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121922\
Data File : BN023279.D
Acq On : 19 Dec 2022 10:45
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 06:26:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 20 06:26:03 2022
Response via : Initial Calibration

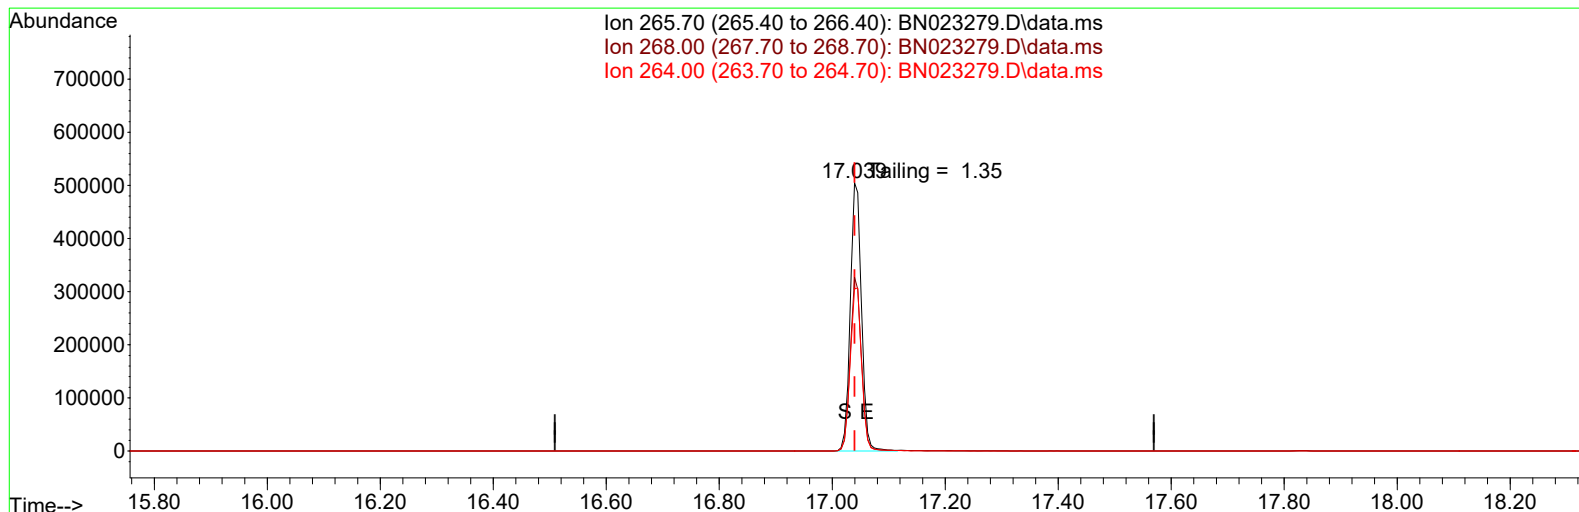

TIC: BN023279.D\data.ms

(70) Pentachlorophenol (C)




17.039min (0.000) 25233.58 ng

response 695470

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.68
264.00	61.60	60.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121922\
 Data File : BN023279.D
 Acq On : 19 Dec 2022 10:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 20 06:26:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 20 06:26:03 2022
 Response via : Initial Calibration

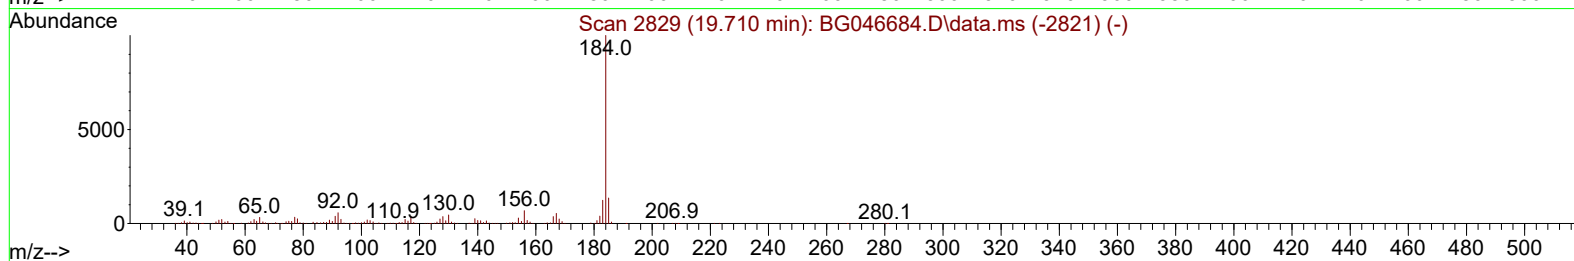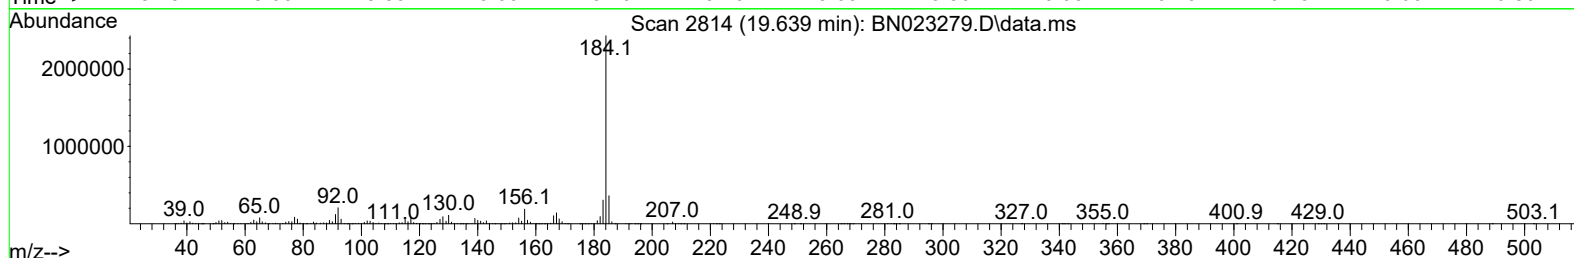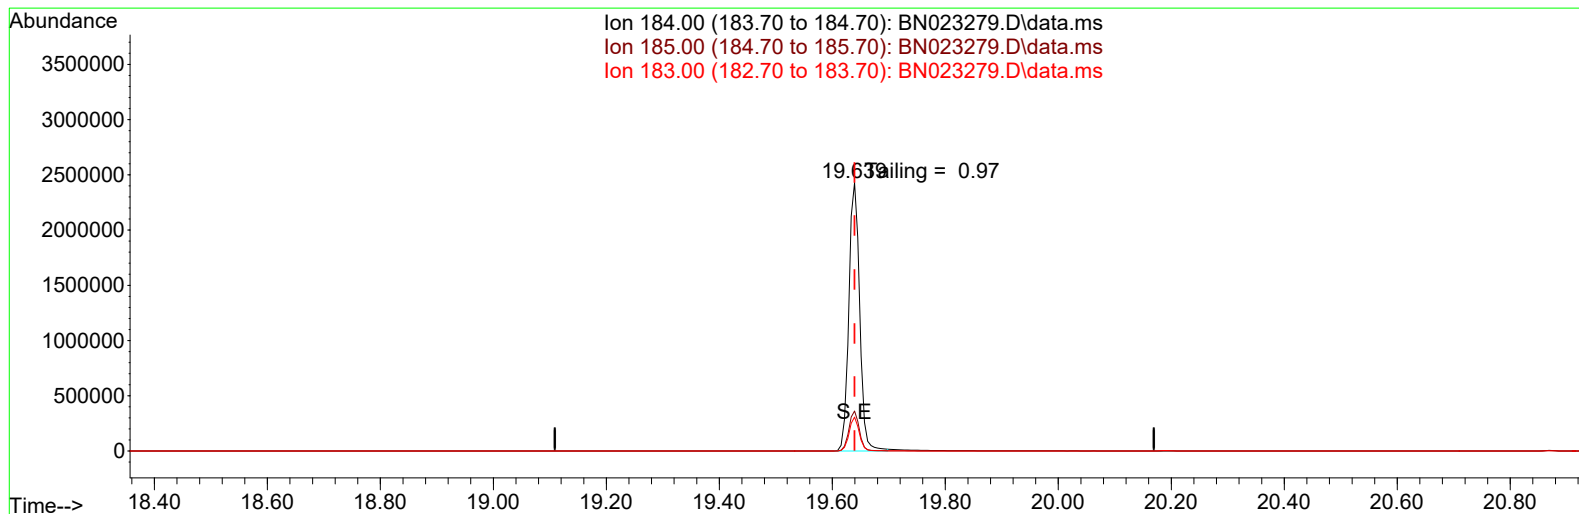

TIC: BN023279.D\data.ms

(77) Benzidine**19.639min (0.000) 579785.01 ng****response 3234848**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.91
183.00	13.20	12.65
0.00	0.00	0.00