
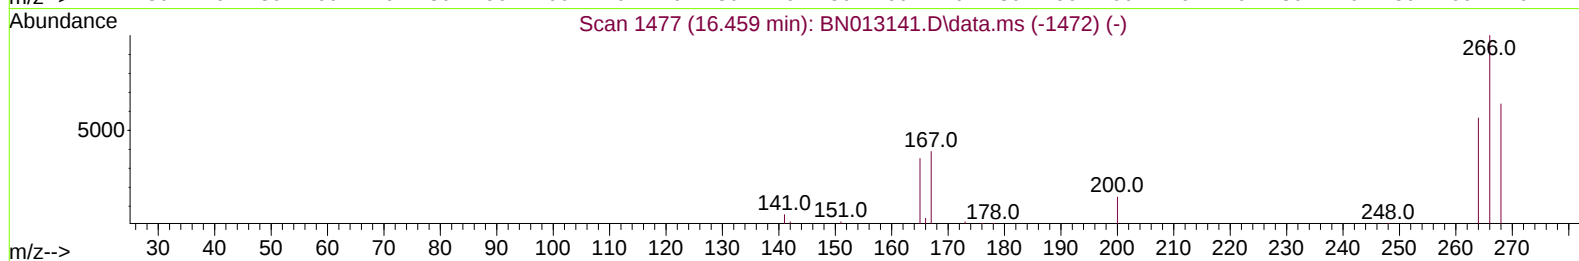
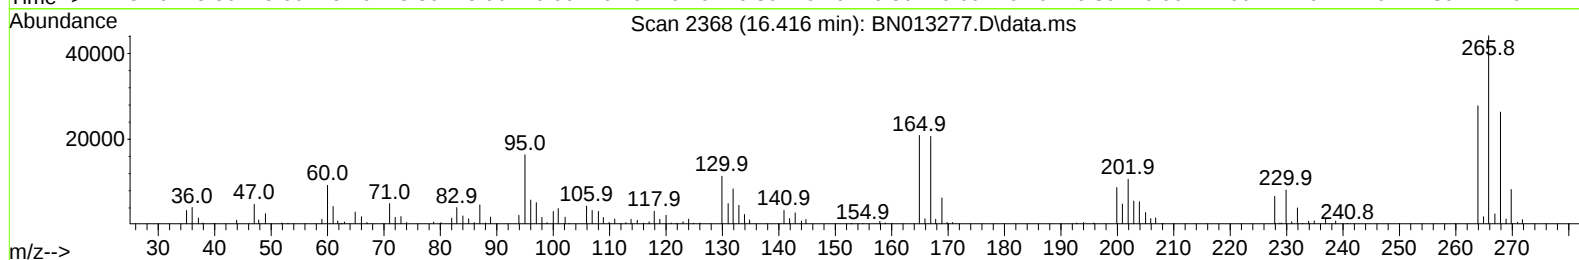


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122320\
 Data File : BN013277.D
 Acq On : 22 Dec 2020 17:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 23 03:23:08 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 22 10:46:43 2020
 Response via : Initial Calibration

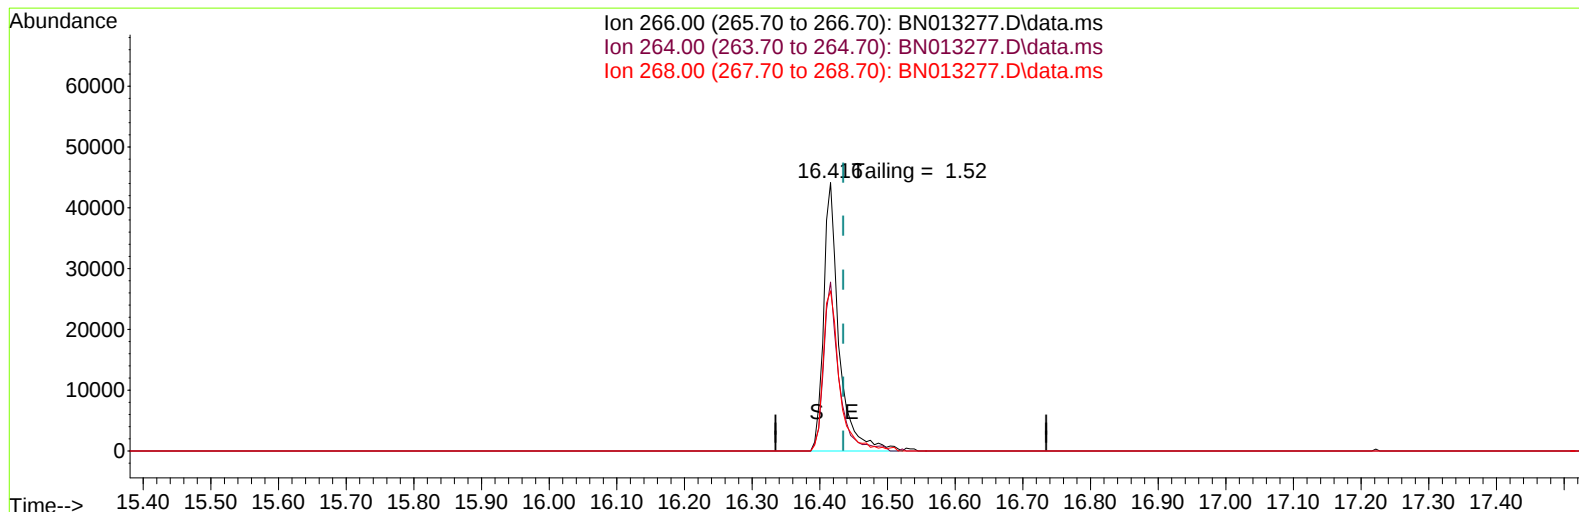

TIC: BN013277.D\data.ms

(24) Pentachlorophenol

16.416min (-0.019) 0.00 ng

response 69849

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.70
268.00	64.40	63.87
0.00	0.00	0.00