
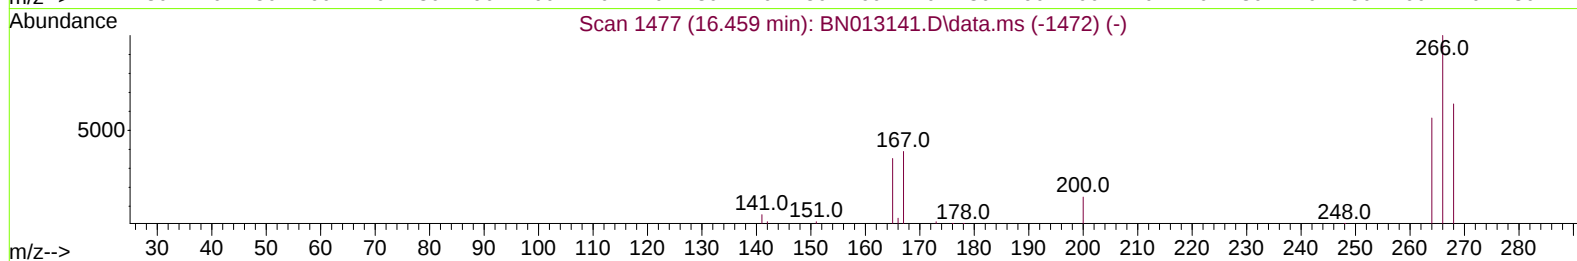
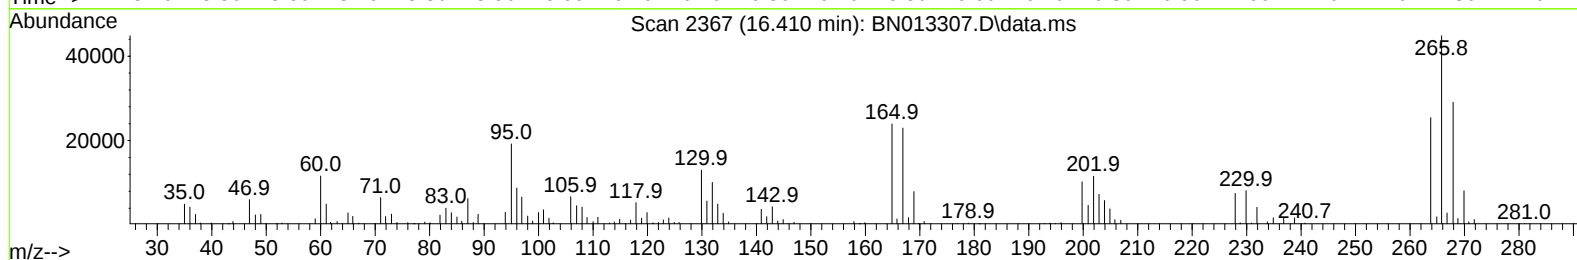


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122320\
 Data File : BN013307.D
 Acq On : 23 Dec 2020 23:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 24 04:50:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 22 10:46:43 2020
 Response via : Initial Calibration

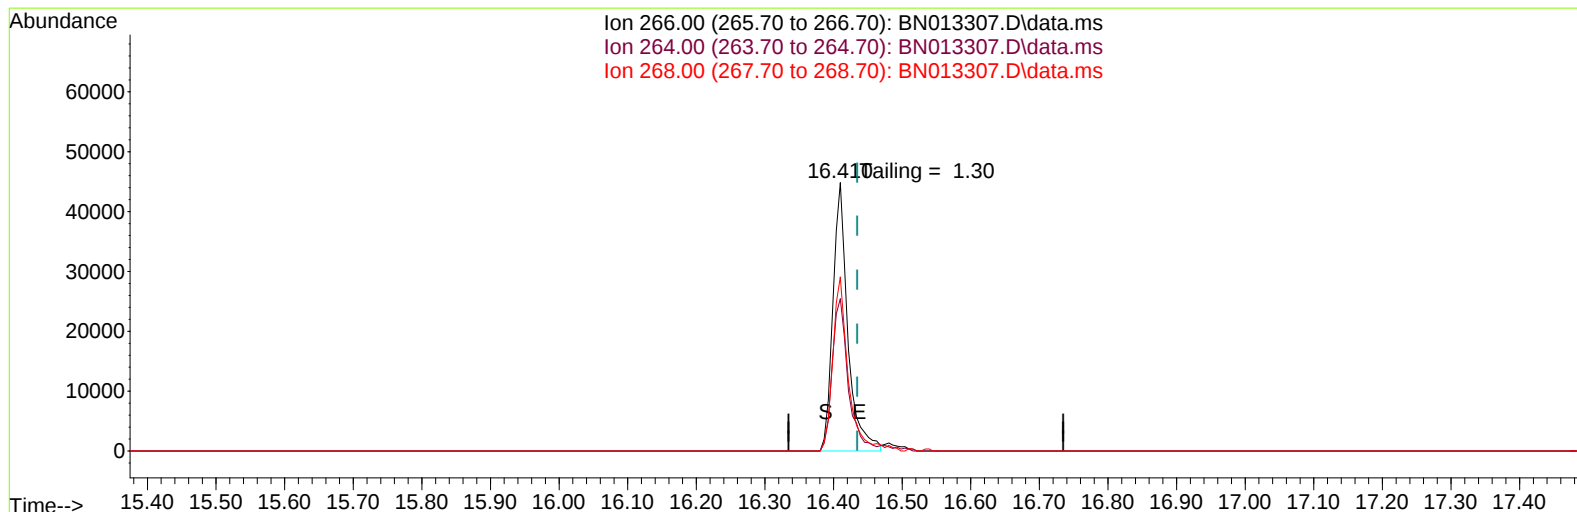

TIC: BN013307.D\data.ms

(24) Pentachlorophenol

16.410min (-0.025) 0.00 ng

response 68316

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	60.15
268.00	64.40	67.26
0.00	0.00	0.00