


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122320\
Data File : BN013277.D
Acq On : 22 Dec 2020 17:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Dec 22 10:46:43 2020

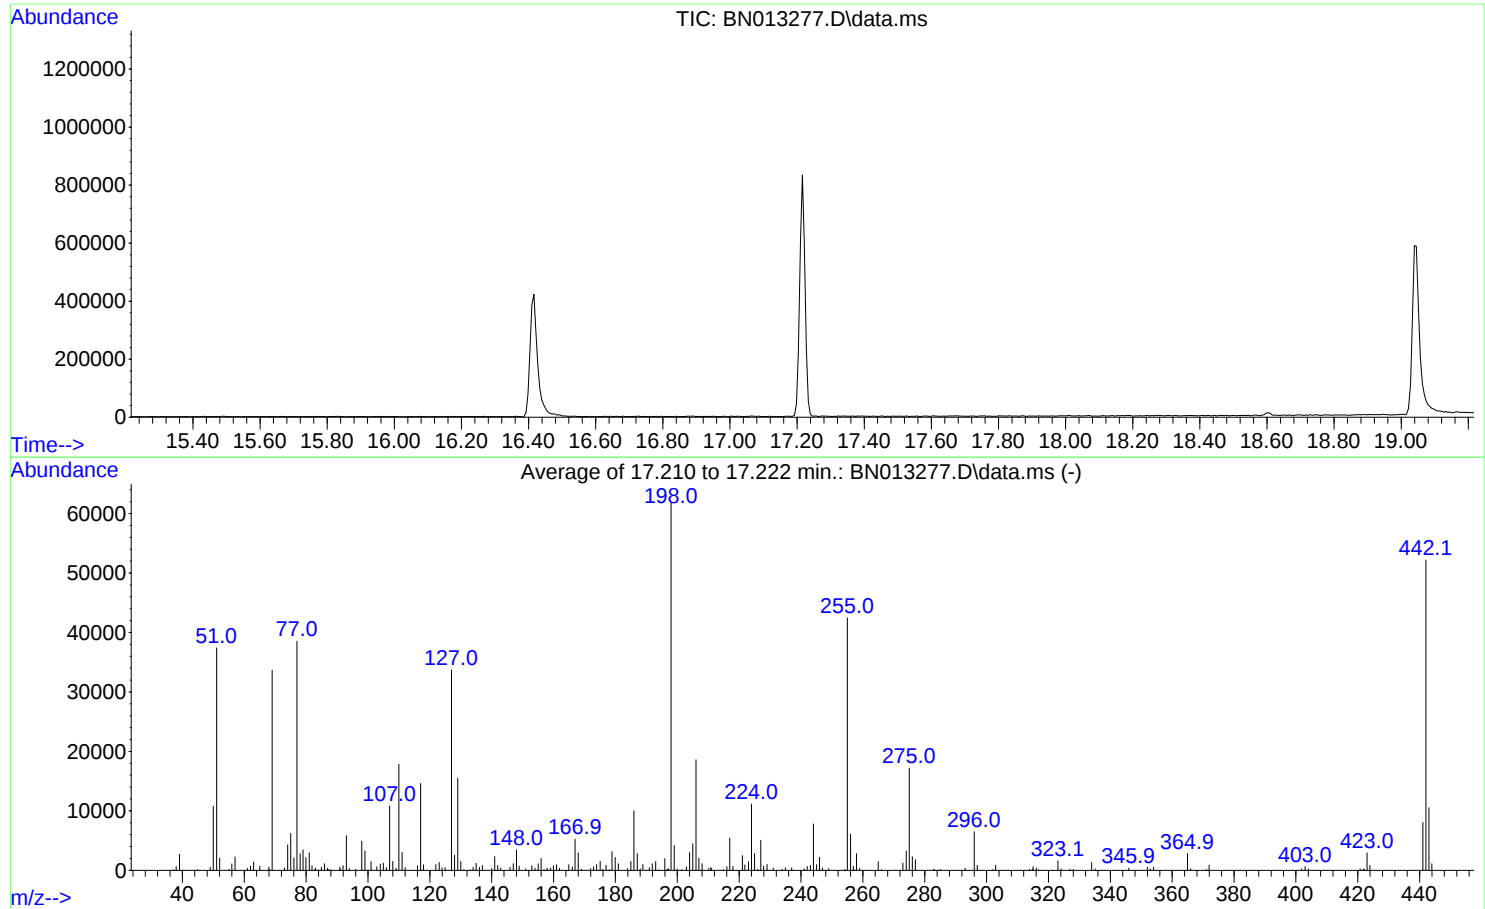

AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.5	37395	PASS
68	69	0.00	2	1.6	551	PASS
69	198	0.00	100	54.4	33640	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.5	33717	PASS
197	198	0.00	2	0.4	239	PASS
198	198	100	100	100.0	61861	PASS
199	198	5	9	6.8	4192	PASS
275	198	10	60	27.8	17188	PASS
365	198	1	100	4.6	2822	PASS
441	198	0.01	100	13.0	8063	PASS
442	442	50	100	100.0	52173	PASS
443	442	15	24	20.2	10540	PASS