


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN122320\
 Data File : BN013307.D
 Acq On : 23 Dec 2020 23:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 22 10:46:43 2020

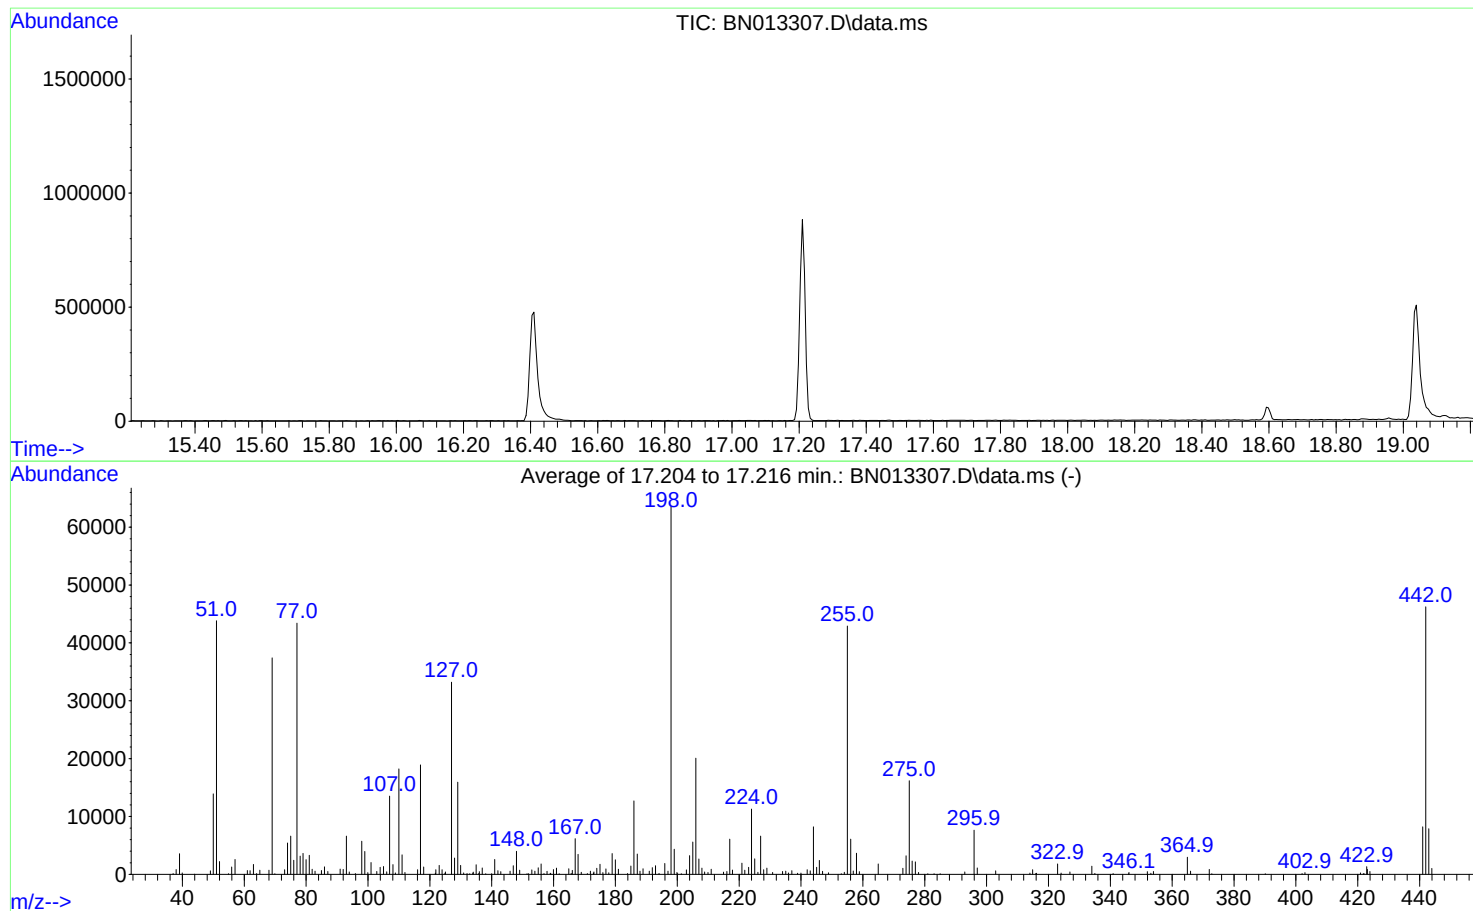

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2496

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	68.9	43821	PASS
68	69	0.00	2	1.9	712	PASS
69	198	0.00	100	58.9	37416	PASS
70	69	0.00	2	0.3	107	PASS
127	198	10	80	52.3	33221	PASS
197	198	0.00	2	0.9	553	PASS
198	198	100	100	100.0	63573	PASS
199	198	5	9	6.8	4343	PASS
275	198	10	60	25.4	16170	PASS
365	198	1	100	4.6	2949	PASS
441	198	0.01	100	12.9	8223	PASS
442	442	50	100	100.0	46237	PASS
443	442	15	24	17.0	7882	PASS