
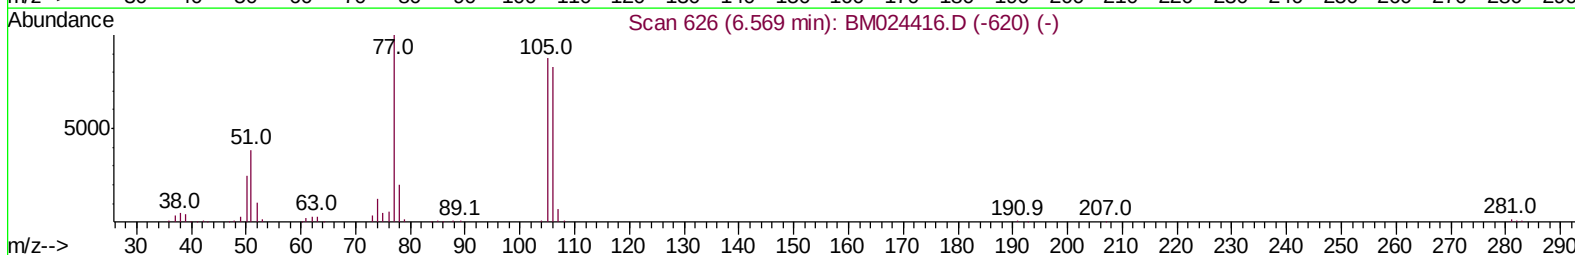
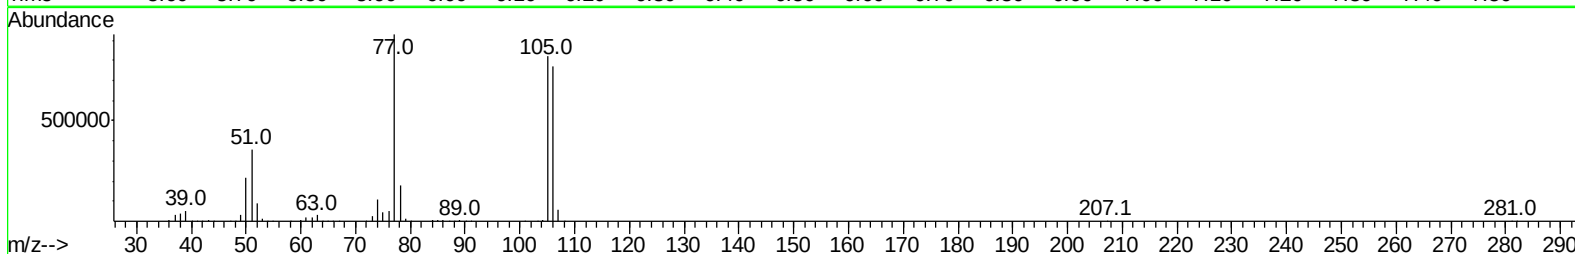


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM010320\
Data File : BM024419.D
Acq On : 03 Jan 2020 18:08
Operator : JU
Sample : SSTD16003
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 03 18:40:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 03 16:57:52 2020
Response via : Initial Calibration

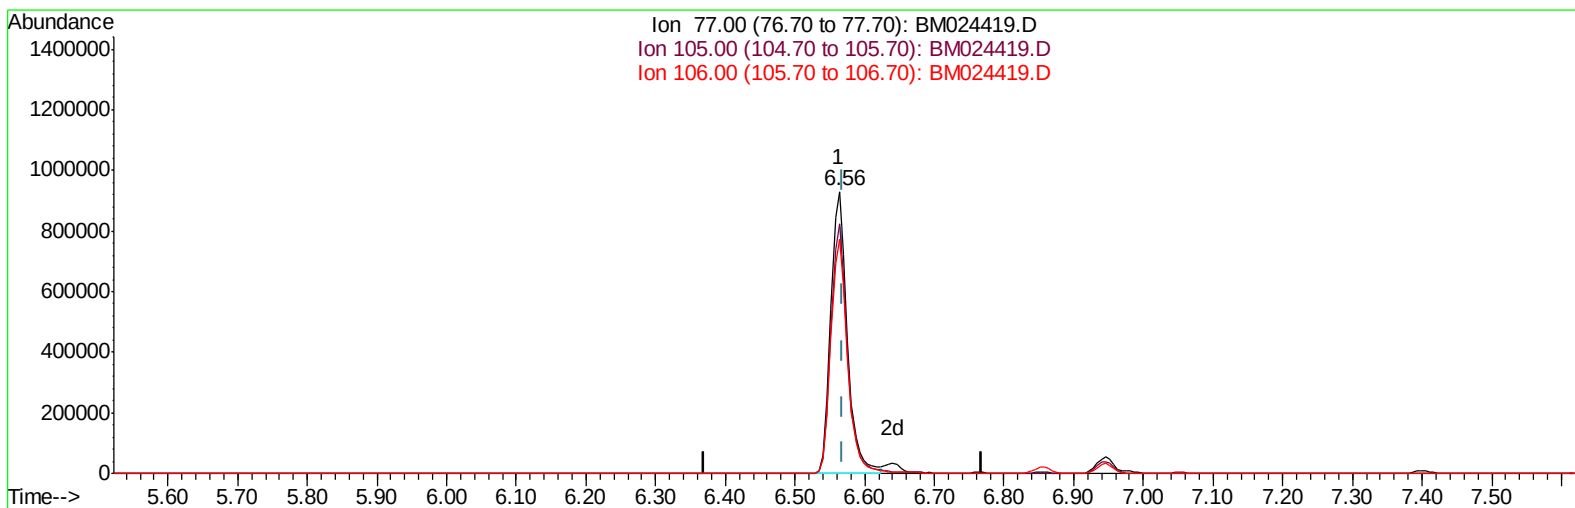

TIC: BM024419.D

(4) Benzaldehyde




6.563min (-0.006) 99.01ng/ul

response 1530034

Ion	Exp%	Act%
77.00	100	100
105.00	88.00	88.64
106.00	83.30	83.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM010320\
Data File : BM024419.D
Acq On : 03 Jan 2020 18:08
Operator : JU
Sample : SSTD16003
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 03 18:40:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 03 16:57:52 2020
Response via : Initial Calibration

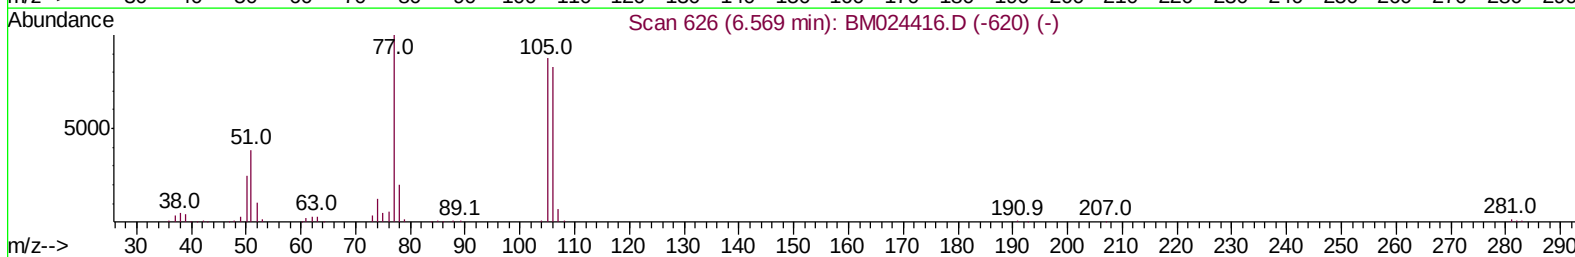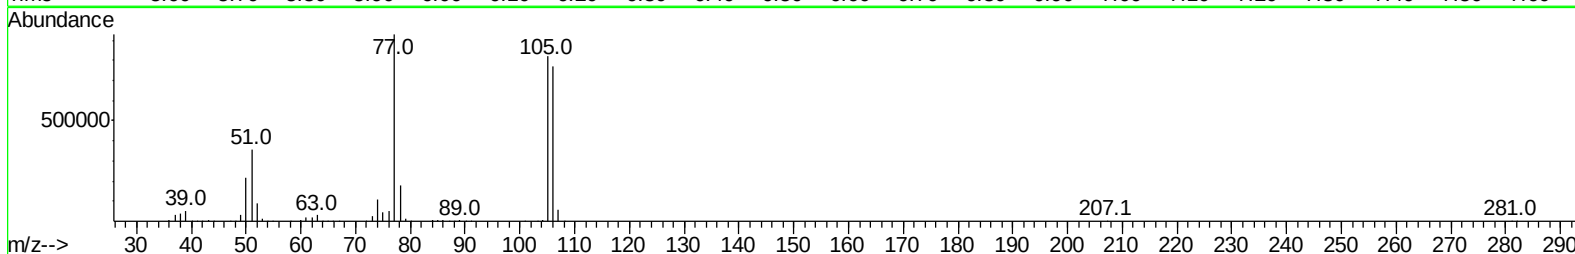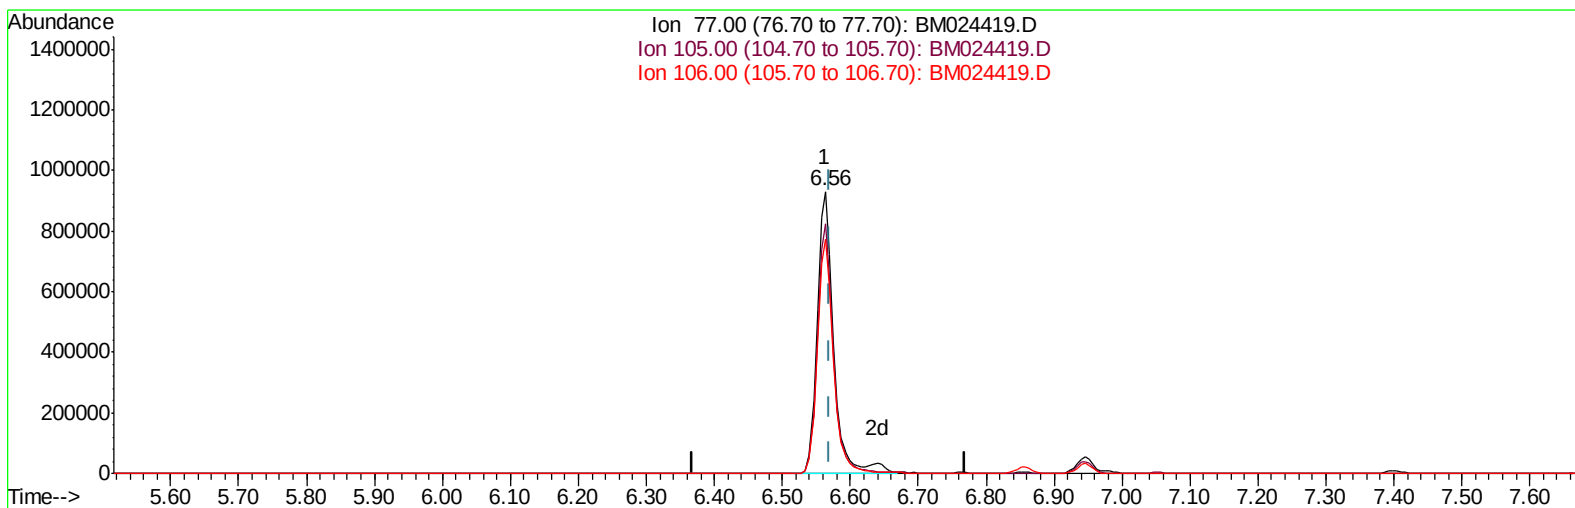

TIC: BM024419.D

(4) Benzaldehyde




6.563min (-0.006) 102.71ng/ul m

response 1587142

Ion	Exp%	Act%
77.00	100	100
105.00	88.00	88.64
106.00	83.30	83.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM010320\
Data File : BM024419.D
Acq On : 03 Jan 2020 18:08
Operator : JU
Sample : SSTD16003
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 03 18:40:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 03 16:57:52 2020
Response via : Initial Calibration

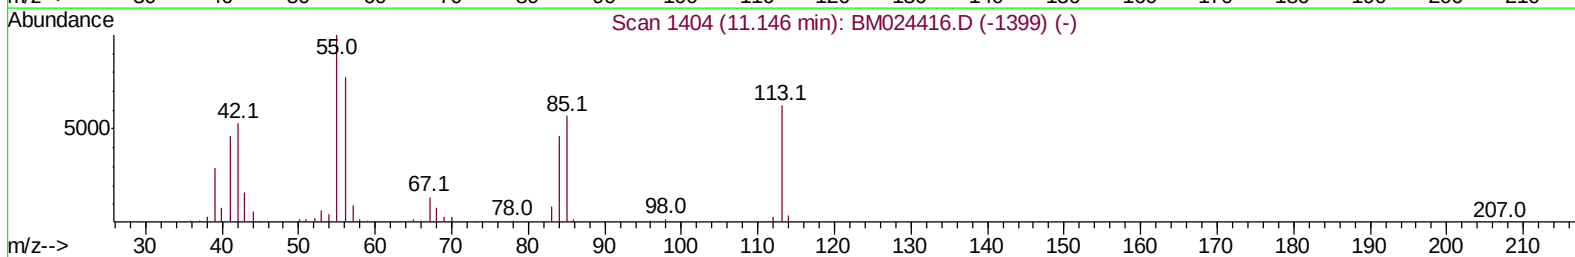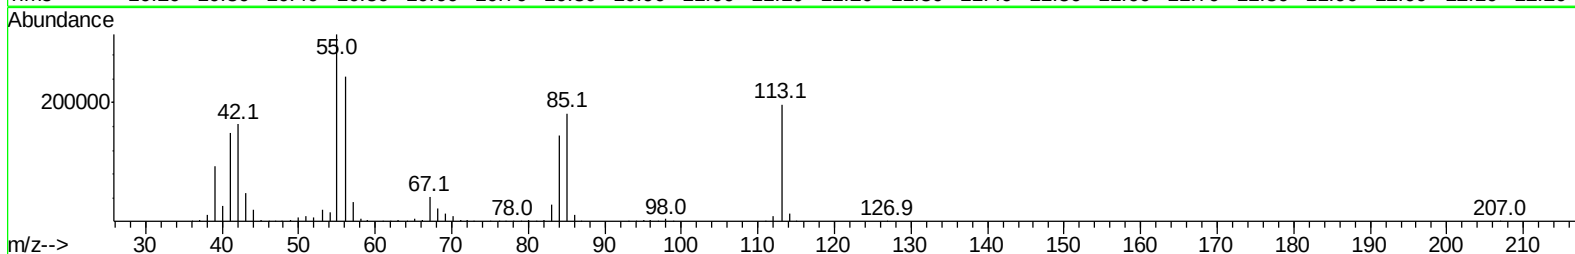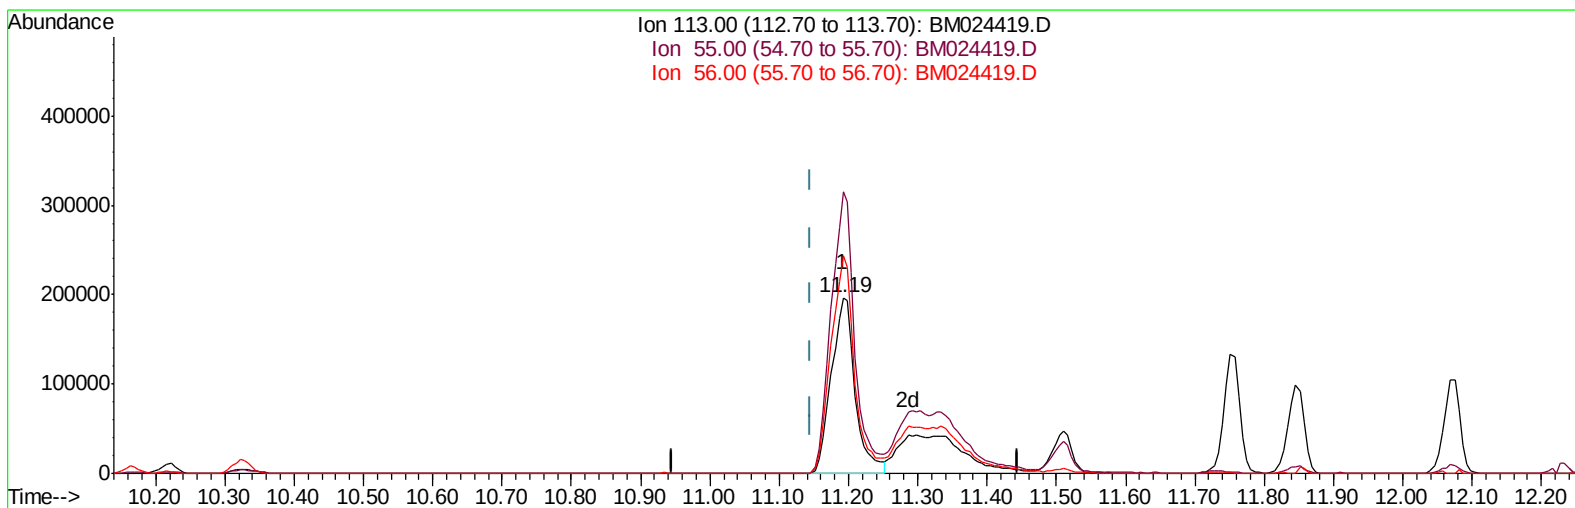

TIC: BM024419.D

(32) Caprolactam




11.193min (+0.047) 78.08ng/ul

response 471145

Ion	Exp%	Act%
113.00	100	100
55.00	161.50	160.10
56.00	123.80	123.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM010320\
Data File : BM024419.D
Acq On : 03 Jan 2020 18:08
Operator : JU
Sample : SSTD16003
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 03 18:40:26 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010320MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 03 16:57:52 2020
Response via : Initial Calibration

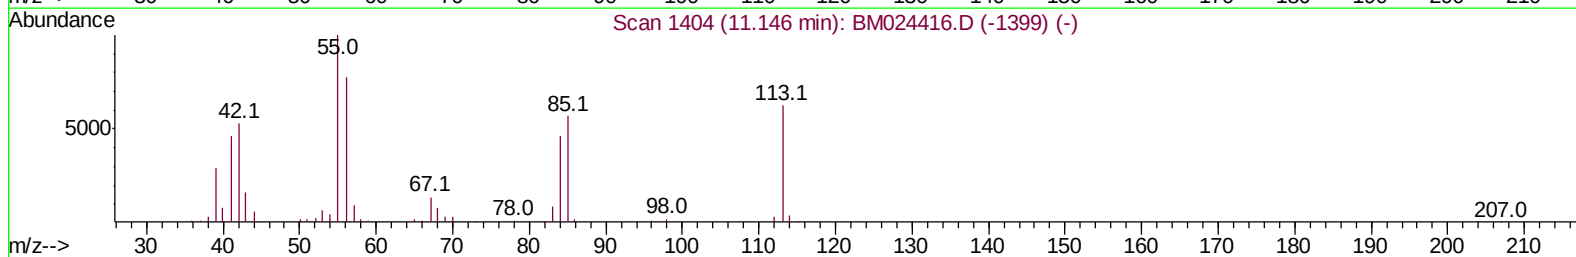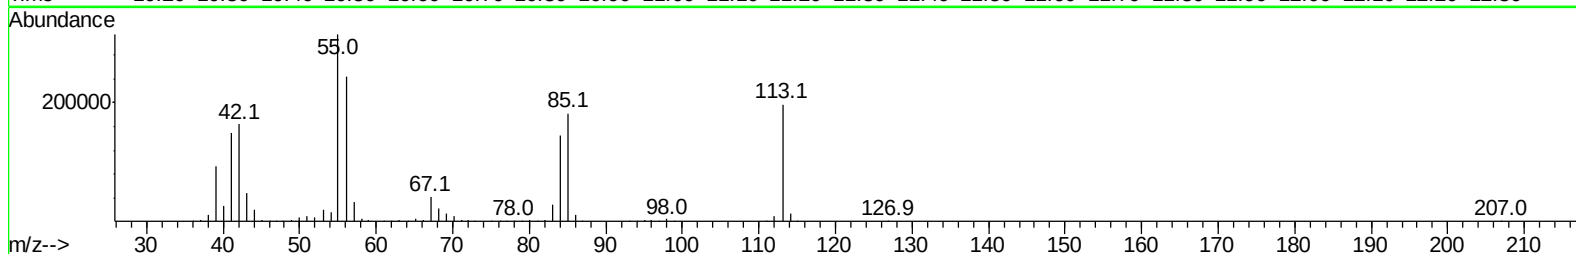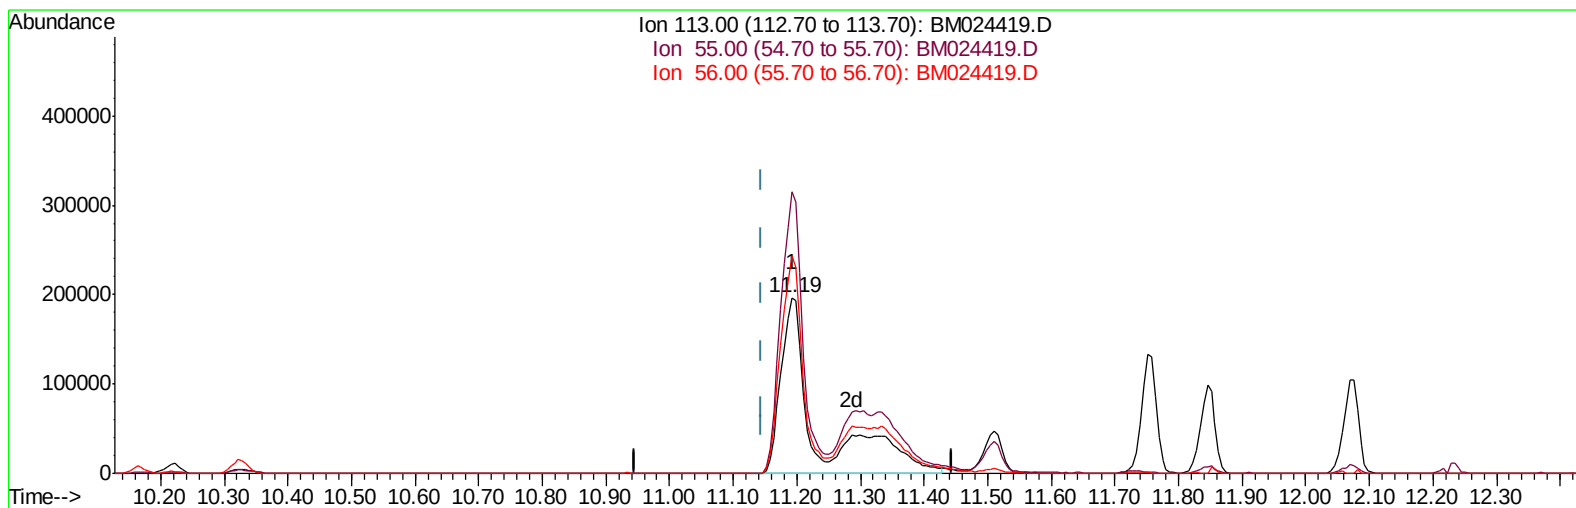

TIC: BM024419.D

(32) Caprolactam

11.193min (+0.047) 124.43ng/ul m

response 750806

Ion	Exp%	Act%
113.00	100	100
55.00	161.50	160.10
56.00	123.80	123.84
0.00	0.00	0.00