

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018353.D
 Acq On : 06 Jan 2022 15:36
 Operator : CG/JU
 Sample : N1026-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG5

Quant Time: Jan 07 09:29:49 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 07 01:31:51 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.593	152	399315	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	1877865	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.234	164	1272392	20.000	ng/ul	0.00
64) Phenanthrene-d10	16.981	188	2664995	20.000	ng/ul	0.00
79) Chrysene-d12	21.174	240	2439973	20.000	ng/ul	# 0.00
88) Perylene-d12	23.392	264	2605617	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.064	96	20227	2.036	ng/uL	0.00
4) Pyridine-d5	3.481	84	70197	2.258	ng/ul	0.02
7) Phenol-d5	6.775	99	314188	8.096	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.934	67	256374	10.371	ng/ul	0.00
11) 2-Chlorophenol-d4	7.128	132	259867	9.142	ng/ul	0.00
15) 4-Methylphenol-d8	8.310	113	249349	8.140	ng/ul	0.00
21) Nitrobenzene-d5	8.740	128	128950	9.220	ng/ul	0.00
24) 2-Nitrophenol-d4	9.463	143	125876	8.420	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.004	165	211254	7.777	ng/ul	0.00
31) 4-Chloroaniline-d4	10.510	131	340296	8.152	ng/ul	0.00
46) Dimethylphthalate-d6	13.651	166	1036286	11.213	ng/ul	0.00
49) Acenaphthylene-d8	13.928	160	1063737	9.105	ng/ul	0.00
54) 4-Nitrophenol-d4	14.457	143	75156	4.262	ng/ul	0.00
60) Fluorene-d10	15.228	176	835684	10.718	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.357	200	77215	5.120	ng/ul	0.00
73) Anthracene-d10	17.075	188	1329952	10.775	ng/ul	0.00
81) Pyrene-d10	19.375	212	1507934	10.773	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.251	264	1251907	9.654	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.410	105	97177	2.071	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018353.D
Acq On : 06 Jan 2022 15:36
Operator : CG/JU
Sample : N1026-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG5

Quant Time: Jan 07 09:29:49 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 07 01:31:51 2022
Response via : Initial Calibration

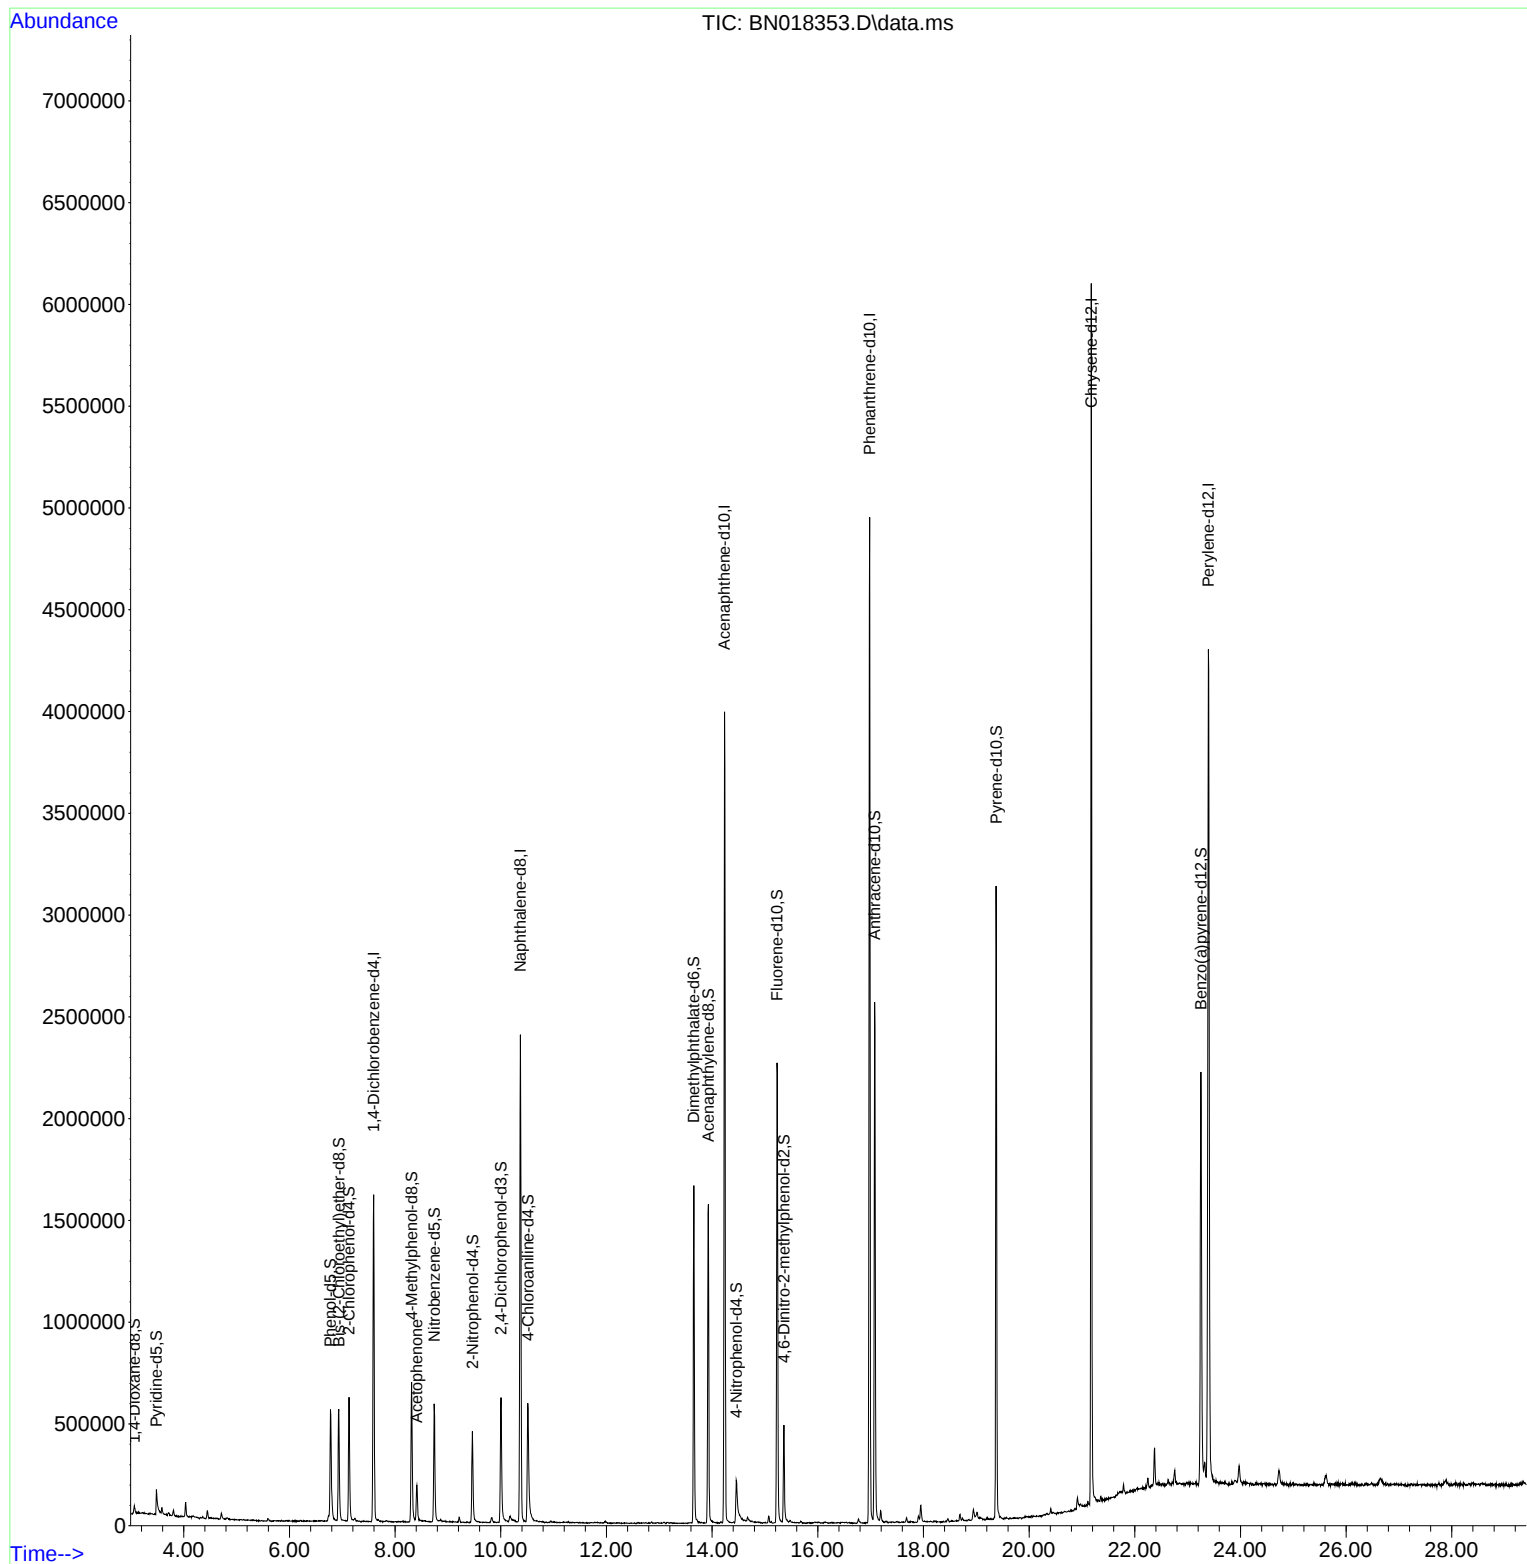

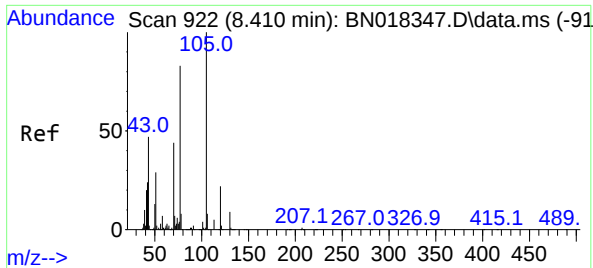

#16
 Acetophenone
 Concen: 2.071 ng/ul
 RT: 8.410 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BN018353.D
 Acq: 06 Jan 2022 15:36

Instrument :
 BNA_N
 ClientSampleId :
 BGLG5

Tgt Ion:105 Resp: 97177

Ion	Ratio	Lower	Upper
105	100		
77	81.5	64.8	97.2
51	32.5	22.8	34.2

