

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018353.D
 Acq On : 06 Jan 2022 15:36
 Operator : CG/JU
 Sample : N1026-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018353.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.064	9	13	19	rVB3	37539	56155	0.74%	0.085%
2	3.481	82	84	94	rBV	123502	221299	2.92%	0.336%
3	3.587	99	102	107	rVB2	32239	43768	0.58%	0.066%
4	3.805	135	139	146	rVB3	30863	44527	0.59%	0.068%
5	4.034	174	178	183	rBV2	69618	84829	1.12%	0.129%
6	4.358	231	233	238	rVB3	9226	9809	0.13%	0.015%
7	4.446	243	248	253	rBV2	39643	64839	0.85%	0.098%
8	4.711	288	293	302	rBV2	30240	49301	0.65%	0.075%
9	4.817	308	311	316	rVB6	7246	11805	0.16%	0.018%
10	5.593	439	443	447	rBV5	12545	20218	0.27%	0.031%
11	6.740	634	638	639	rBV	25211	28909	0.38%	0.044%
12	6.775	639	644	655	rVB	541065	968932	12.77%	1.471%
13	6.934	664	671	680	rBV	546854	903556	11.90%	1.372%
14	7.128	697	704	713	rBV	609030	986534	13.00%	1.498%
15	7.240	717	723	726	rVB6	12984	24531	0.32%	0.037%
16	7.593	775	783	795	rBV	1607762	2589885	34.12%	3.933%
17	7.669	795	796	802	rVB6	9383	13458	0.18%	0.020%
18	8.310	898	905	916	rBV	686484	1135099	14.95%	1.724%
19	8.410	916	922	931	rVV	177526	329225	4.34%	0.500%
20	8.475	931	933	938	rVB5	5001	8449	0.11%	0.013%
21	8.740	971	978	990	rBV	579585	991100	13.06%	1.505%
22	9.210	1053	1058	1063	rVB3	24547	37153	0.49%	0.056%
23	9.463	1095	1101	1116	rBV	446930	781383	10.29%	1.187%
24	9.828	1158	1163	1171	rBV5	24163	50612	0.67%	0.077%
25	10.004	1186	1193	1203	rBV	613294	1074855	14.16%	1.632%
26	10.175	1216	1222	1228	rBV6	29597	71440	0.94%	0.108%
27	10.369	1246	1255	1266	rBV	2394275	4036263	53.18%	6.129%
28	10.510	1273	1279	1296	rBV	582246	1225644	16.15%	1.861%
29	10.640	1299	1301	1307	rVV7	7053	13930	0.18%	0.021%
30	10.681	1307	1308	1315	rVB6	7061	9949	0.13%	0.015%
31	10.946	1348	1353	1354	rBV5	7381	9023	0.12%	0.014%
32	11.275	1406	1409	1413	rVB6	7582	8919	0.12%	0.014%
33	11.981	1522	1529	1530	rBV5	11460	16821	0.22%	0.026%
34	11.993	1530	1531	1537	rVB4	6579	7904	0.10%	0.012%
35	12.593	1627	1633	1634	rBV5	5786	8758	0.12%	0.013%
36	12.851	1671	1677	1680	rBV4	7935	10988	0.14%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018353.D
 Acq On : 06 Jan 2022 15:36
 Operator : CG/JU
 Sample : N1026-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG5

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

37	13.087	1711	1717	1722	rVB7	7030	14265	0.19%	0.022%
38	13.651	1807	1813	1821	rBV	1658692	2378559	31.34%	3.612%
39	13.928	1853	1860	1867	rBV	1565403	2338773	30.81%	3.551%
40	14.169	1896	1901	1905	rBV5	9113	15034	0.20%	0.023%
41	14.234	1905	1912	1927	rBV	3986090	5823128	76.72%	8.842%
42	14.404	1938	1941	1944	rVB4	6076	8456	0.11%	0.013%
43	14.457	1944	1950	1968	rBV	211552	607974	8.01%	0.923%
44	14.669	1983	1986	1995	rVV6	22020	43549	0.57%	0.066%
45	15.069	2049	2054	2059	rBV3	34022	54346	0.72%	0.083%
46	15.116	2059	2062	2066	rVB6	8800	10659	0.14%	0.016%
47	15.228	2075	2081	2092	rBV	2259270	3324250	43.80%	5.048%
48	15.357	2098	2103	2112	rBV	476299	717605	9.45%	1.090%
49	15.475	2118	2123	2127	rVB8	9619	15838	0.21%	0.024%
50	15.675	2153	2157	2164	rVB6	10899	22283	0.29%	0.034%
51	16.769	2337	2343	2346	rBV3	22186	34495	0.45%	0.052%
52	16.981	2372	2379	2390	rBV	4941011	6965345	91.76%	10.577%
53	17.075	2390	2395	2410	rVV2	2553243	3667610	48.32%	5.569%
54	17.186	2410	2414	2420	rVB5	51270	79929	1.05%	0.121%
55	17.681	2493	2498	2504	rVB4	23293	32402	0.43%	0.049%
56	17.904	2532	2536	2539	rBV6	29679	43495	0.57%	0.066%
57	17.951	2539	2544	2553	rVB2	79543	140246	1.85%	0.213%
58	18.198	2583	2586	2589	rBV5	7865	10581	0.14%	0.016%
59	18.463	2626	2631	2635	rVB4	15355	24625	0.32%	0.037%
60	18.692	2665	2670	2674	rBV2	32026	46990	0.62%	0.071%
61	18.733	2675	2677	2682	rVB6	13426	16871	0.22%	0.026%
62	18.863	2694	2699	2701	rBV5	6880	9037	0.12%	0.014%
63	18.945	2707	2713	2718	rBV7	52256	106647	1.41%	0.162%
64	19.010	2722	2724	2732	rVB	32250	50791	0.67%	0.077%
65	19.339	2775	2780	2781	rBV5	13250	15424	0.20%	0.023%
66	19.375	2781	2786	2798	rVB	3105800	4156800	54.76%	6.312%
67	20.245	2931	2934	2935	rBV3	7371	7732	0.10%	0.012%
68	20.410	2959	2962	2965	rBV4	23006	21648	0.29%	0.033%
69	20.533	2980	2983	2984	rBV3	10691	11256	0.15%	0.017%
70	20.916	3044	3048	3051	rBV4	56876	88743	1.17%	0.135%
71	21.110	3079	3081	3085	rBV4	22698	30016	0.40%	0.046%
72	21.174	3087	3092	3102	rBV	5999996	7292464	96.07%	11.074%
73	21.357	3120	3123	3127	rBV5	24066	31007	0.41%	0.047%
74	21.786	3193	3196	3199	rBV4	38777	41214	0.54%	0.063%
75	22.374	3291	3296	3301	rVB	180288	249860	3.29%	0.379%
76	22.757	3357	3361	3370	rVB3	68867	114323	1.51%	0.174%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018353.D
Acq On : 06 Jan 2022 15:36
Operator : CG/JU
Sample : N1026-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG5

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Title : SVOA CALIBRATION

77	23.251	3438	3445	3453	rBV	2017755	3650368	48.09%	5.543%
78	23.392	3462	3469	3482	rVB2	4070630	7590416	100.00%	11.526%


Sum of corrected areas: 65854924

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018353.D
Acq On : 06 Jan 2022 15:36
Operator : CG/JU
Sample : N1026-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

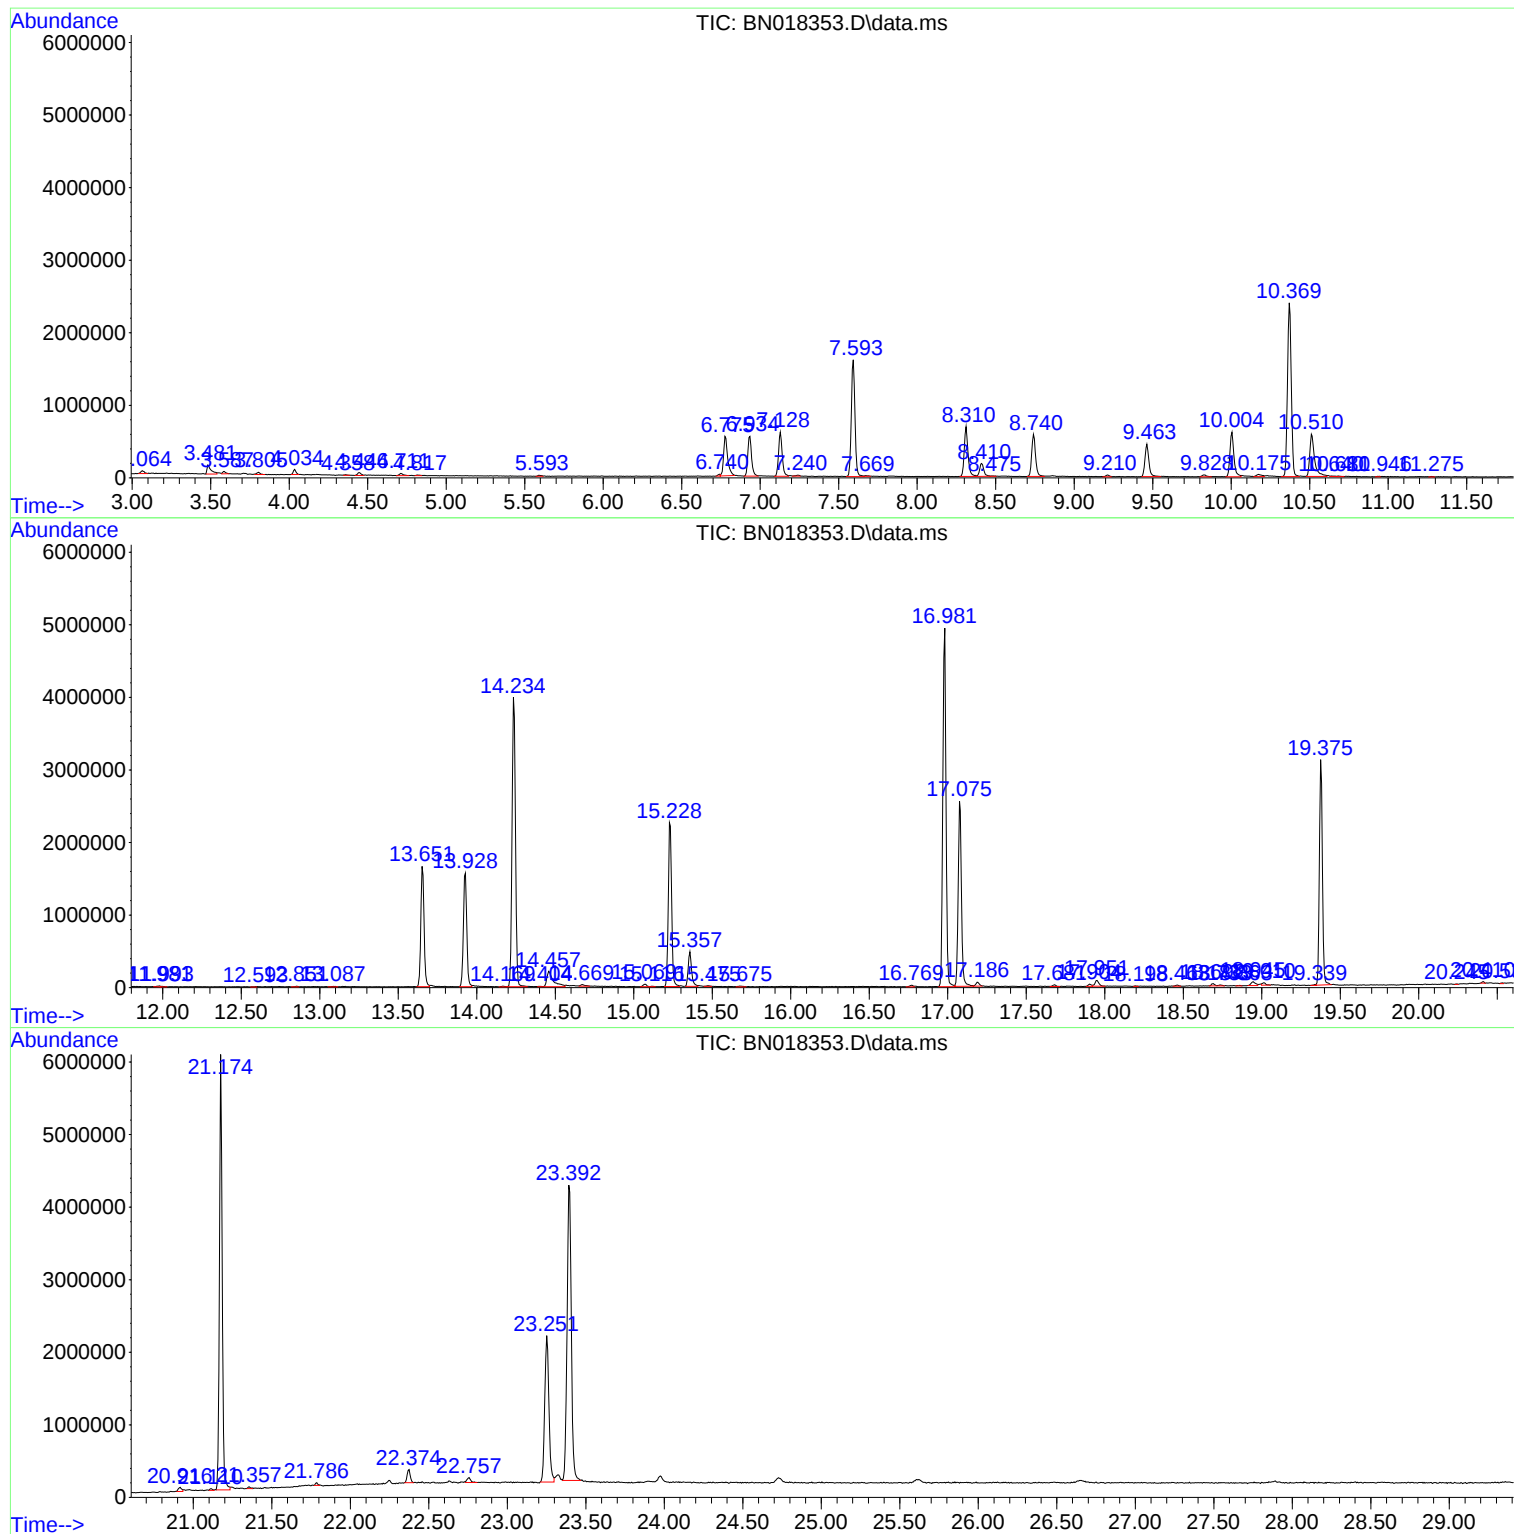

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018353.D
Acq On : 06 Jan 2022 15:36
Operator : CG/JU
Sample : N1026-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018353.D
Acq On : 06 Jan 2022 15:36
Operator : CG/JU
Sample : N1026-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------