

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018354.D
 Acq On : 06 Jan 2022 16:19
 Operator : CG/JU
 Sample : N1026-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018354.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	9	12	22	rBV	42546	71024	0.90%	0.094%
2	3.705	119	122	129	rVB7	16234	28726	0.36%	0.038%
3	3.799	134	138	145	rVB2	28004	44260	0.56%	0.059%
4	4.452	247	249	252	rVB4	7653	8294	0.10%	0.011%
5	4.711	289	293	302	rVB3	34293	63860	0.80%	0.085%
6	6.775	637	644	659	rVV	646825	1093673	13.79%	1.448%
7	6.928	664	670	683	rVV	695697	1079361	13.61%	1.429%
8	7.122	697	703	715	rBV	712433	1172765	14.78%	1.553%
9	7.228	719	721	726	rVB6	11089	17643	0.22%	0.023%
10	7.587	775	782	793	rBV	1627519	2589751	32.64%	3.430%
11	7.663	793	795	801	rVB7	10397	20345	0.26%	0.027%
12	8.305	898	904	919	rBV	769730	1364324	17.20%	1.807%
13	8.416	919	923	929	rVB4	17391	33361	0.42%	0.044%
14	8.740	971	978	988	rBV	693902	1182660	14.91%	1.566%
15	9.210	1052	1058	1065	rBV2	25436	42180	0.53%	0.056%
16	9.340	1074	1080	1084	rVB3	10885	17986	0.23%	0.024%
17	9.463	1094	1101	1119	rBV	514378	903564	11.39%	1.197%
18	9.999	1186	1192	1216	rBV	701488	1330063	16.77%	1.761%
19	10.169	1216	1221	1226	rBV5	27996	48728	0.61%	0.065%
20	10.369	1247	1255	1272	rBV	2394419	4027506	50.77%	5.334%
21	10.510	1272	1279	1303	rBV	715883	1423848	17.95%	1.886%
22	11.981	1523	1529	1537	rVB5	10926	25033	0.32%	0.033%
23	12.851	1672	1677	1682	rVB7	7032	10730	0.14%	0.014%
24	13.087	1712	1717	1719	rBV5	8302	13080	0.16%	0.017%
25	13.157	1724	1729	1735	rVV5	8691	17532	0.22%	0.023%
26	13.651	1807	1813	1826	rBV	2000432	2876416	36.26%	3.809%
27	13.922	1853	1859	1874	rBV	1857068	2888053	36.40%	3.825%
28	14.169	1895	1901	1905	rVB5	9531	12622	0.16%	0.017%
29	14.234	1905	1912	1924	rBV	3849438	5653865	71.27%	7.488%
30	14.457	1945	1950	1966	rBV3	200431	567246	7.15%	0.751%
31	14.675	1983	1987	1991	rVB5	19082	31440	0.40%	0.042%
32	14.963	2035	2036	2043	rVB7	6534	8093	0.10%	0.011%
33	15.069	2048	2054	2059	rBV2	37421	61231	0.77%	0.081%
34	15.116	2059	2062	2067	rVB4	14301	18728	0.24%	0.025%
35	15.234	2075	2082	2097	rBV	2735786	4108979	51.80%	5.442%
36	15.357	2097	2103	2115	rVV2	353554	573724	7.23%	0.760%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018354.D
 Acq On : 06 Jan 2022 16:19
 Operator : CG/JU
 Sample : N1026-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

37	15.475	2120	2123	2126	rVB4	12474	14145	0.18%	0.019%
38	15.534	2131	2133	2137	rVB4	10716	9437	0.12%	0.012%
39	15.604	2143	2145	2147	rBV3	7685	8176	0.10%	0.011%
40	15.681	2154	2158	2164	rVB9	14858	25554	0.32%	0.034%
41	15.940	2201	2202	2205	rVV3	9153	9822	0.12%	0.013%
42	15.981	2205	2209	2210	rVV4	13211	15517	0.20%	0.021%
43	16.004	2210	2213	2222	rVB9	21015	43723	0.55%	0.058%
44	16.769	2339	2343	2346	rBV2	31506	50166	0.63%	0.066%
45	16.828	2349	2353	2359	rVB7	17594	30052	0.38%	0.040%
46	16.981	2373	2379	2389	rBV	4708198	6835547	86.16%	9.053%
47	17.075	2389	2395	2410	rVV2	3048040	4643244	58.53%	6.149%
48	17.192	2411	2415	2421	rVV7	38795	70953	0.89%	0.094%
49	17.239	2421	2423	2428	rVB6	7976	10296	0.13%	0.014%
50	17.434	2451	2456	2460	rBV8	14042	28129	0.35%	0.037%
51	17.592	2481	2483	2488	rVB6	16927	21806	0.27%	0.029%
52	17.681	2493	2498	2505	rVB3	38284	62410	0.79%	0.083%
53	17.904	2533	2536	2537	rBV3	19174	17786	0.22%	0.024%
54	18.057	2559	2562	2568	rVB8	40281	53197	0.67%	0.070%
55	18.345	2609	2611	2615	rVB5	21266	28234	0.36%	0.037%
56	18.675	2663	2667	2668	rBV4	15665	18373	0.23%	0.024%
57	18.945	2706	2713	2718	rVB7	52198	107076	1.35%	0.142%
58	19.016	2721	2725	2730	rBV2	55136	82863	1.04%	0.110%
59	19.375	2781	2786	2793	rBV	3989533	5333607	67.23%	7.063%
60	19.963	2884	2886	2889	rVB3	35702	31331	0.39%	0.041%
61	20.916	3044	3048	3055	rBV2	187016	310035	3.91%	0.411%
62	21.116	3080	3082	3085	rVB3	62814	62205	0.78%	0.082%
63	21.175	3087	3092	3105	rVV	5345592	7396577	93.24%	9.795%
64	21.357	3121	3123	3127	rVB2	80585	79338	1.00%	0.105%
65	21.786	3193	3196	3204	rVB2	126484	160166	2.02%	0.212%
66	22.251	3271	3275	3282	rVB2	211497	261502	3.30%	0.346%
67	22.757	3357	3361	3366	rBV	296305	427407	5.39%	0.566%
68	23.257	3439	3446	3453	rBV2	2781278	5224235	65.85%	6.919%
69	23.327	3454	3458	3463	rVV2	413665	736872	9.29%	0.976%
70	23.398	3463	3470	3482	rVB2	4061532	7933128	100.00%	10.506%
71	23.980	3563	3569	3576	rVB	371465	702760	8.86%	0.931%
72	24.733	3692	3697	3706	rVB	308437	665759	8.39%	0.882%
73	25.621	3843	3848	3861	rVB3	235101	567887	7.16%	0.752%




Sum of corrected areas: 75510009

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018354.D
Acq On : 06 Jan 2022 16:19
Operator : CG/JU
Sample : N1026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

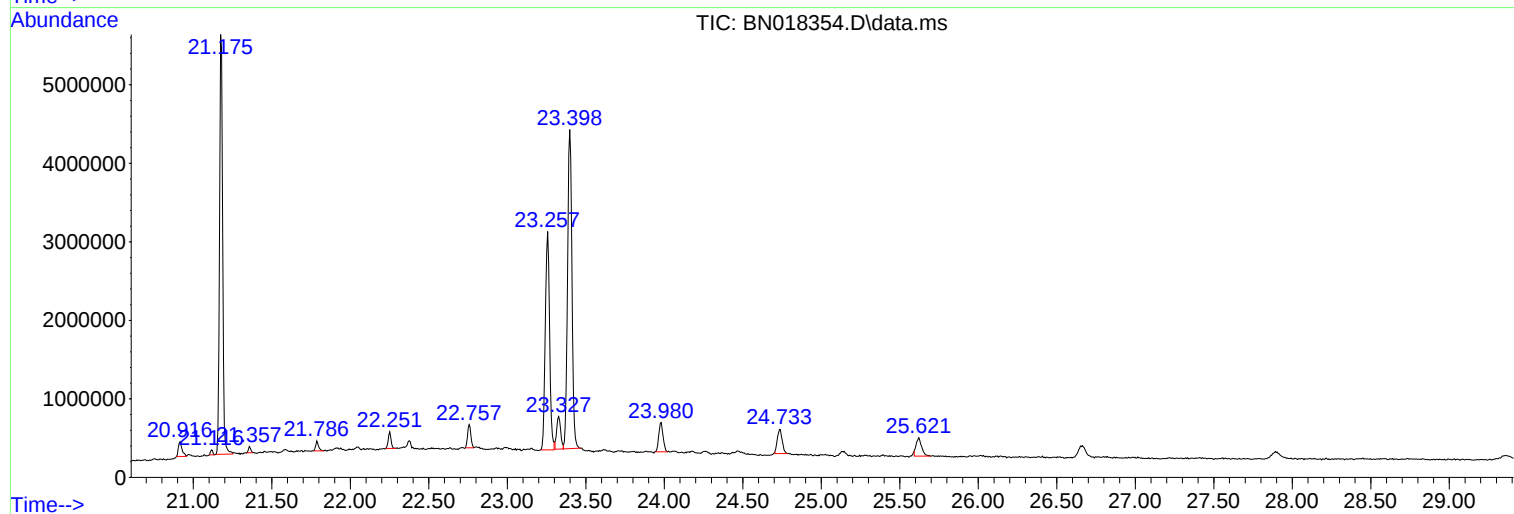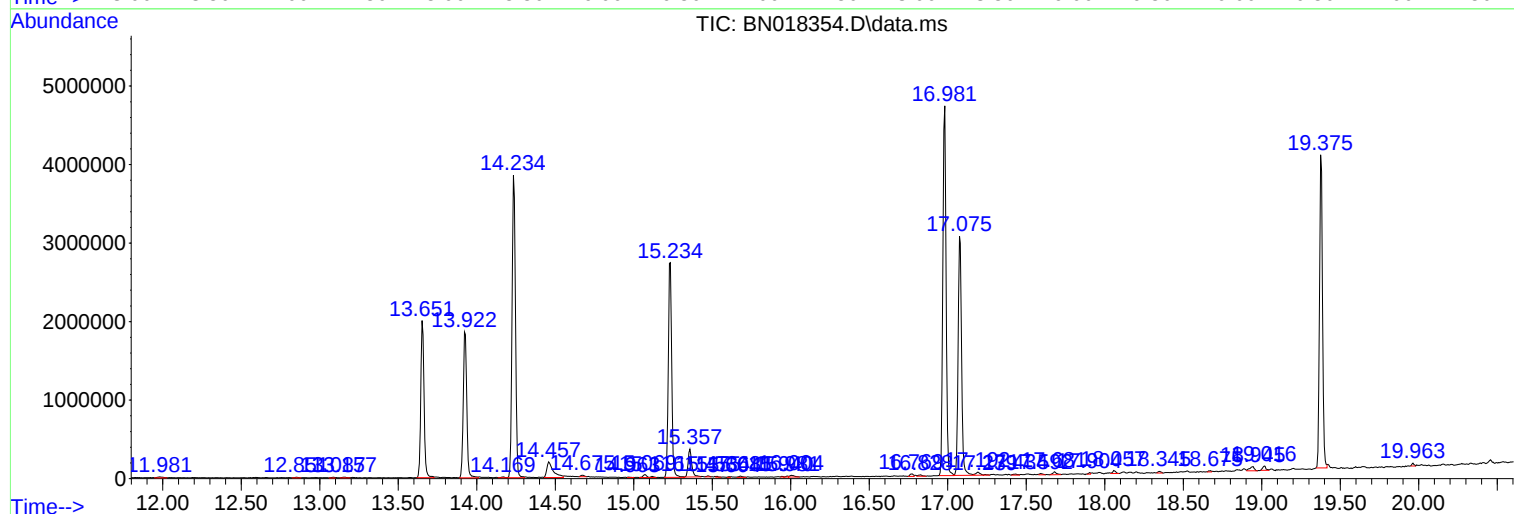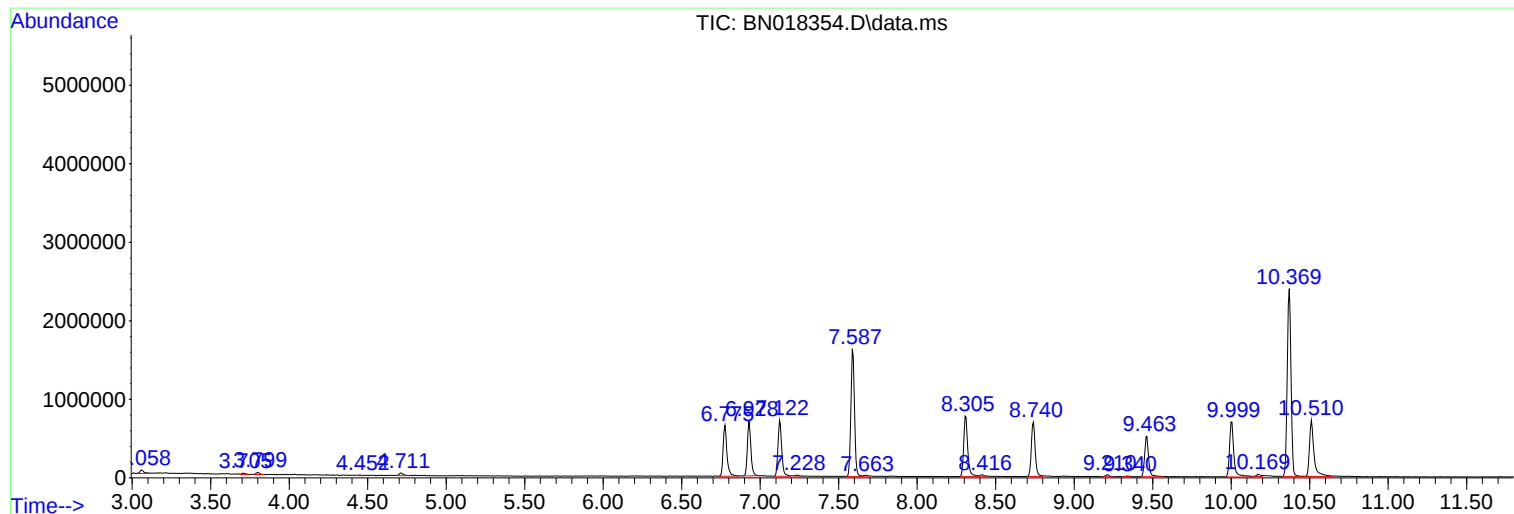

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018354.D
Acq On : 06 Jan 2022 16:19
Operator : CG/JU
Sample : N1026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018354.D
Acq On : 06 Jan 2022 16:19
Operator : CG/JU
Sample : N1026-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG6

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------