

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018355.D
 Acq On : 06 Jan 2022 16:55
 Operator : CG/JU
 Sample : N1026-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018355.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.717	119	124	129	rBV6	14251	22826	0.31%	0.065%
2	3.805	135	139	143	rVB4	26982	41983	0.56%	0.119%
3	4.711	289	293	301	rBV3	28647	56708	0.76%	0.161%
4	7.246	718	724	728	rBV6	8955	14829	0.20%	0.042%
5	7.593	777	783	799	rBV	1412817	2369077	31.80%	6.740%
6	7.740	805	808	817	rVB8	4876	12111	0.16%	0.034%
7	8.293	900	902	905	rVB3	6408	7619	0.10%	0.022%
8	10.369	1246	1255	1270	rBV	2049479	3651231	49.01%	10.387%
9	14.234	1906	1912	1929	rBV	3515942	5330202	71.54%	15.164%
10	15.081	2050	2056	2061	rBV	34622	59620	0.80%	0.170%
11	16.769	2338	2343	2347	rBV3	14828	21350	0.29%	0.061%
12	16.981	2372	2379	2394	rBV	4267649	6501460	87.27%	18.496%
13	17.175	2410	2412	2424	rVB7	7500	18130	0.24%	0.052%
14	17.975	2544	2548	2550	rVB3	7141	7779	0.10%	0.022%
15	18.992	2719	2721	2726	rVB5	8985	13336	0.18%	0.038%
16	19.345	2777	2781	2784	rBV4	7806	9542	0.13%	0.027%
17	21.174	3086	3092	3103	rBV	5394504	7182796	96.41%	20.434%
18	21.351	3119	3122	3128	rBV6	29973	54716	0.73%	0.156%
19	21.786	3193	3196	3199	rVB2	57311	63483	0.85%	0.181%
20	22.245	3270	3274	3279	rBV2	119292	165116	2.22%	0.470%
21	22.751	3356	3360	3365	rVB3	181245	263025	3.53%	0.748%
22	23.321	3452	3457	3462	rBV	268290	437366	5.87%	1.244%
23	23.392	3462	3469	3482	rVB	3848582	7450156	100.00%	21.195%
24	23.974	3562	3568	3576	rVB	268147	527750	7.08%	1.501%
25	24.727	3689	3696	3705	rVB3	213495	499321	6.70%	1.420%
26	25.604	3841	3845	3856	rVB4	143863	369738	4.96%	1.052%




Sum of corrected areas: 35151270

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018355.D
Acq On : 06 Jan 2022 16:55
Operator : CG/JU
Sample : N1026-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

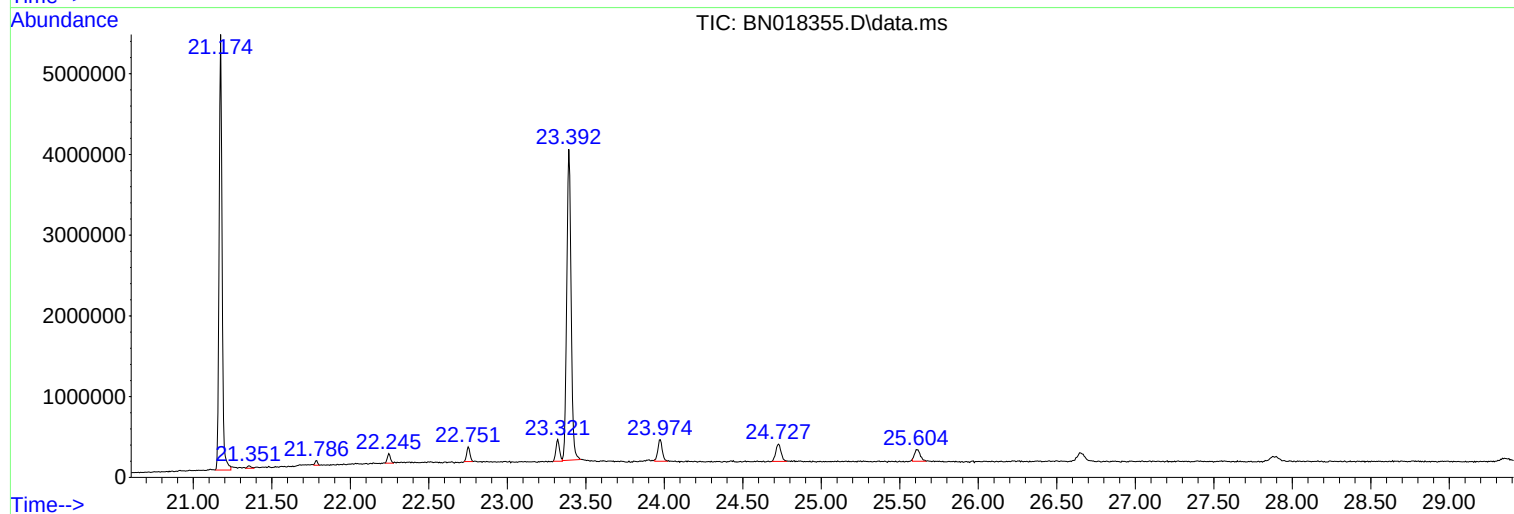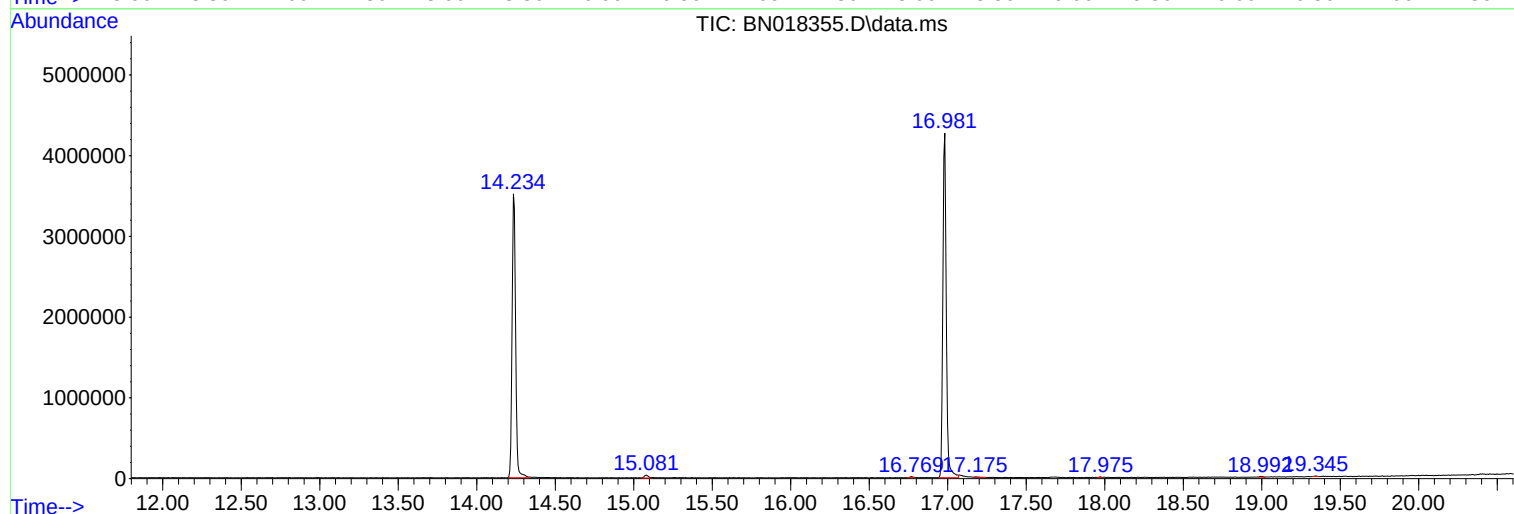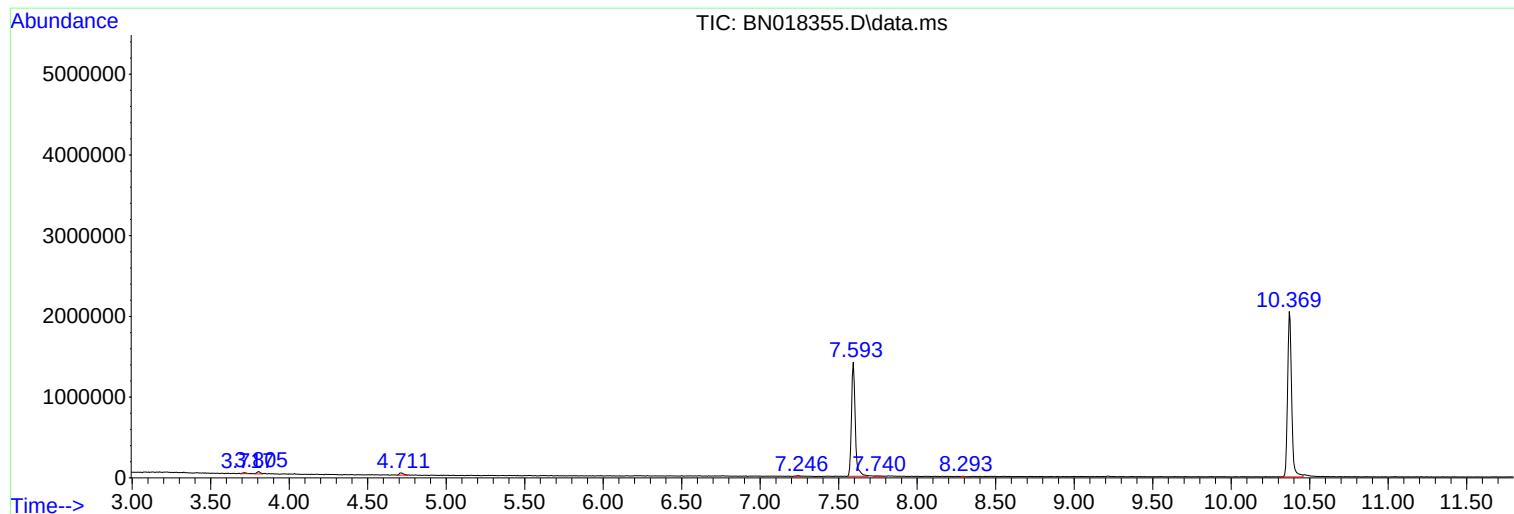

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018355.D
Acq On : 06 Jan 2022 16:55
Operator : CG/JU
Sample : N1026-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018355.D
Acq On : 06 Jan 2022 16:55
Operator : CG/JU
Sample : N1026-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc