

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018356.D
 Acq On : 06 Jan 2022 17:30
 Operator : CG/JU
 Sample : N1026-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018356.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.711	121	123	127	rBV3	8006	10341	0.13%	0.029%
2	3.805	135	139	147	rVB2	25349	42338	0.54%	0.118%
3	4.717	290	294	300	rVB3	23891	43784	0.56%	0.122%
4	7.234	719	722	727	rBV4	8464	12162	0.15%	0.034%
5	7.593	776	783	802	rBV	1454292	2458365	31.27%	6.848%
6	10.375	1248	1256	1270	rBV	2047170	3718682	47.30%	10.359%
7	14.240	1905	1913	1932	rBV	3478189	5461190	69.46%	15.213%
8	15.081	2052	2056	2062	rBV2	24493	40400	0.51%	0.113%
9	16.769	2337	2343	2347	rBV3	11897	18817	0.24%	0.052%
10	16.981	2372	2379	2393	rBV	4339959	6677234	84.92%	18.601%
11	19.345	2778	2781	2784	rBV4	9096	13046	0.17%	0.036%
12	20.916	3046	3048	3050	rBV3	11386	13436	0.17%	0.037%
13	21.175	3086	3092	3107	rBV	5448118	7474871	95.07%	20.823%
14	21.786	3193	3196	3199	rVB4	48136	53840	0.68%	0.150%
15	22.245	3270	3274	3278	rBV2	108767	131500	1.67%	0.366%
16	22.751	3356	3360	3367	rVB	154939	245504	3.12%	0.684%
17	23.322	3452	3457	3461	rBV2	248220	383052	4.87%	1.067%
18	23.392	3462	3469	3483	rVB	4121253	7862566	100.00%	21.903%
19	23.969	3562	3567	3576	rVB	236838	476667	6.06%	1.328%
20	24.727	3690	3696	3703	rVB	201341	428081	5.44%	1.193%
21	25.615	3841	3847	3856	rVB5	130347	331799	4.22%	0.924%




Sum of corrected areas: 35897675

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018356.D
Acq On : 06 Jan 2022 17:30
Operator : CG/JU
Sample : N1026-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

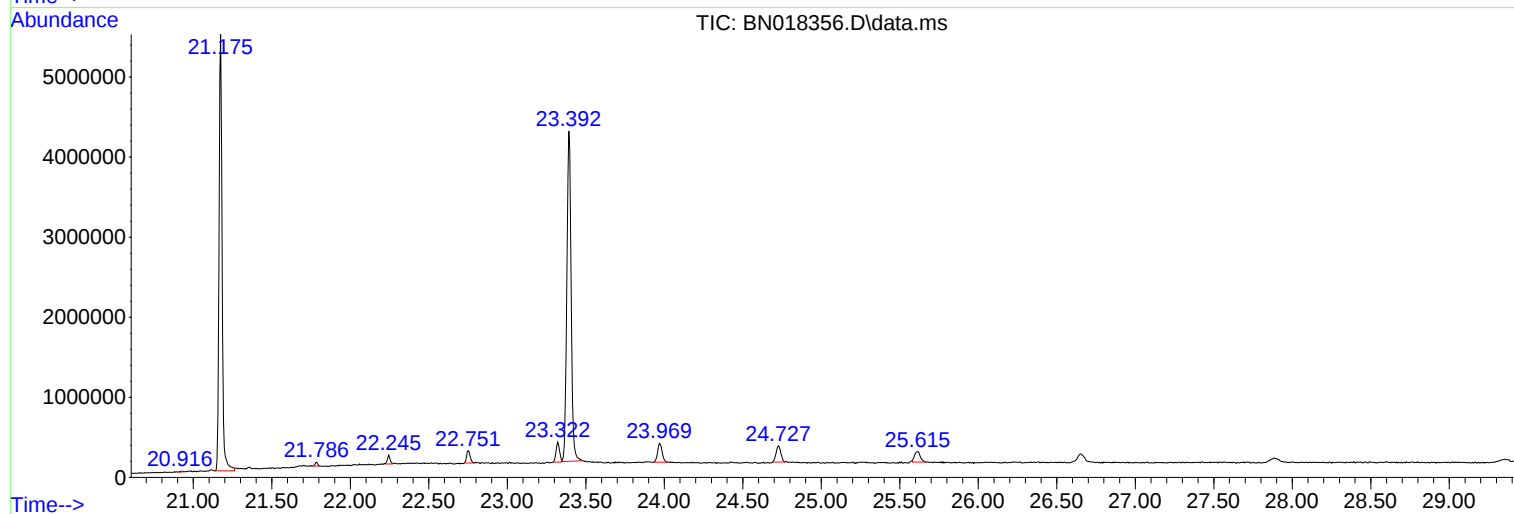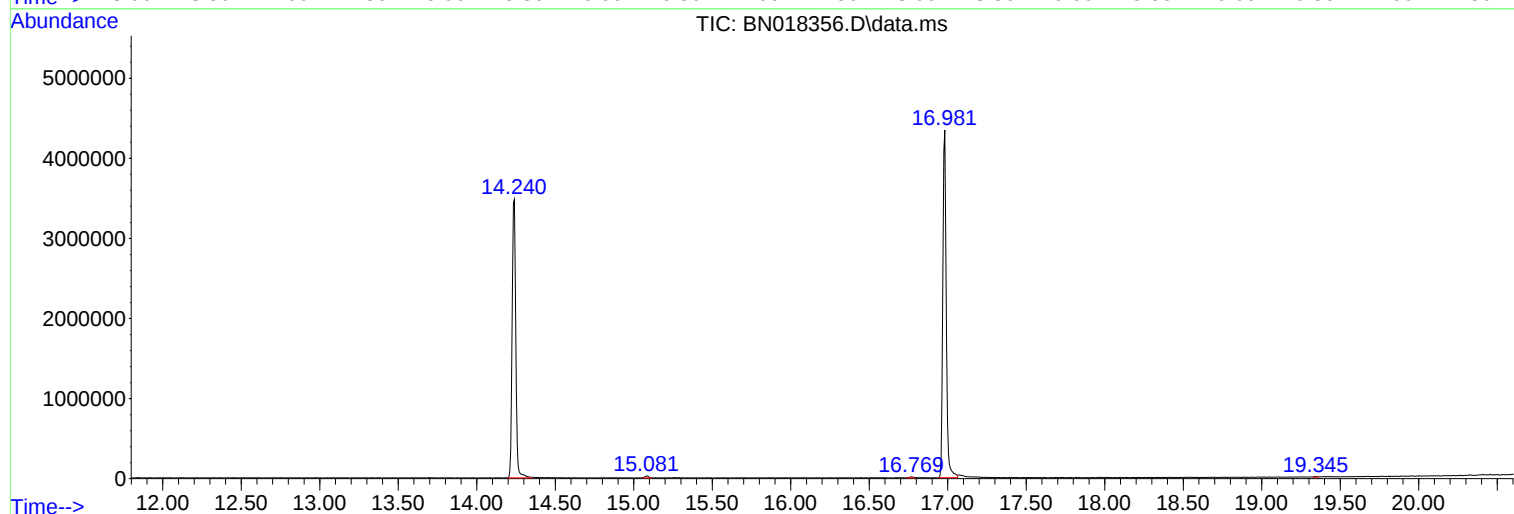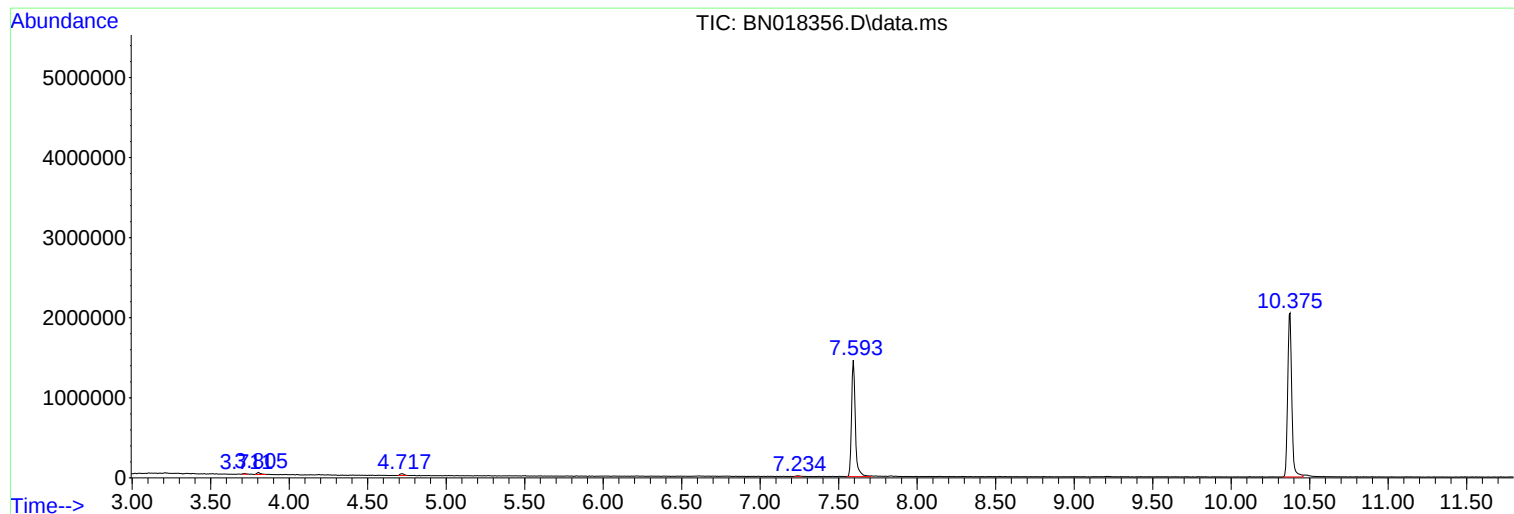

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018356.D
Acq On : 06 Jan 2022 17:30
Operator : CG/JU
Sample : N1026-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018356.D
Acq On : 06 Jan 2022 17:30
Operator : CG/JU
Sample : N1026-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc