

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
 Data File : BN018357.D
 Acq On : 06 Jan 2022 18:06
 Operator : CG/JU
 Sample : N1026-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BGLG9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018357.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.805	136	139	142	rBV2	19482	19572	0.25%	0.054%
2	4.716	290	294	297	rBV	17332	21954	0.28%	0.061%
3	7.240	718	723	729	rBV7	9810	14910	0.19%	0.041%
4	7.593	776	783	796	rBV	1556432	2530630	32.24%	7.040%
5	10.375	1248	1256	1269	rBV	2149827	3832721	48.82%	10.662%
6	10.475	1271	1273	1279	rVB3	16096	23259	0.30%	0.065%
7	14.239	1906	1913	1929	rBV	3558224	5631767	71.74%	15.667%
8	15.081	2051	2056	2062	rBV2	20867	32283	0.41%	0.090%
9	16.775	2339	2344	2351	rVB3	14336	22889	0.29%	0.064%
10	16.980	2372	2379	2402	rBV	4646619	6981549	88.93%	19.422%
11	19.345	2778	2781	2785	rVB5	7555	10430	0.13%	0.029%
12	20.974	3056	3058	3062	rBV5	16919	18700	0.24%	0.052%
13	21.110	3079	3081	3082	rBV2	18620	10376	0.13%	0.029%
14	21.174	3086	3092	3113	rBV	5647322	7564935	96.36%	21.045%
15	21.780	3193	3195	3200	rVB4	39173	50056	0.64%	0.139%
16	22.251	3271	3275	3281	rVB4	74260	108835	1.39%	0.303%
17	22.751	3356	3360	3364	rBV3	122735	185399	2.36%	0.516%
18	23.321	3452	3457	3462	rBV3	181618	302365	3.85%	0.841%
19	23.392	3462	3469	3484	rVB	4181573	7850334	100.00%	21.839%
20	23.974	3562	3568	3577	rVB3	187175	405199	5.16%	1.127%
21	24.727	3691	3696	3704	rVB2	157339	328577	4.19%	0.914%




Sum of corrected areas: 35946740

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018357.D
Acq On : 06 Jan 2022 18:06
Operator : CG/JU
Sample : N1026-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

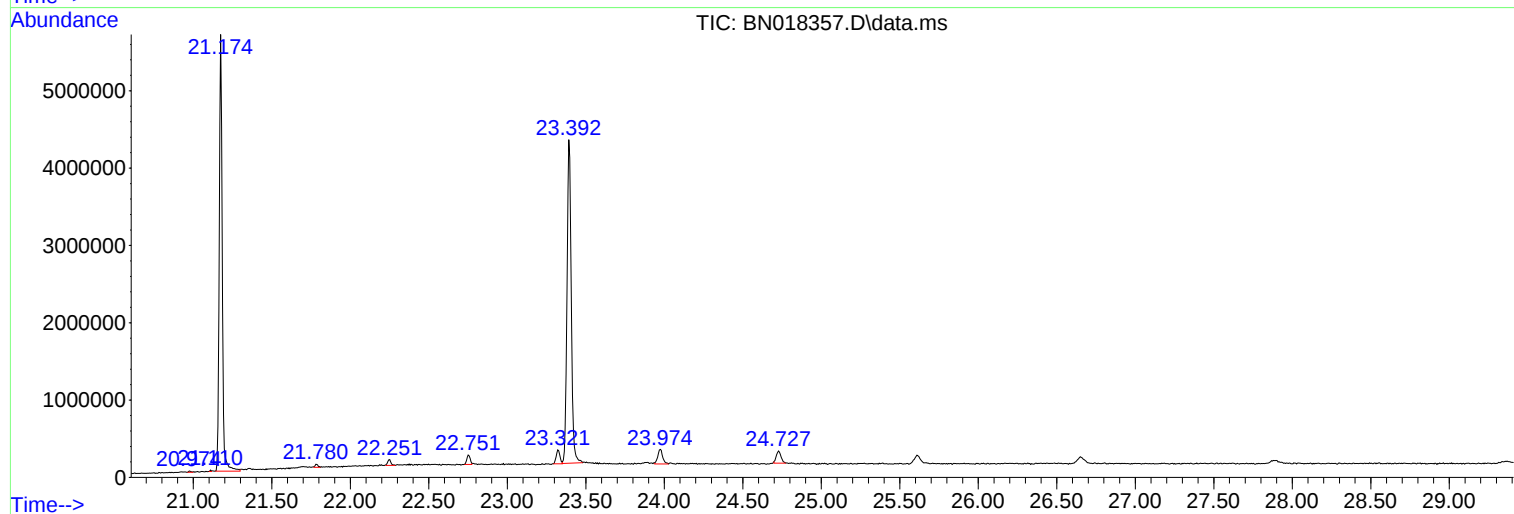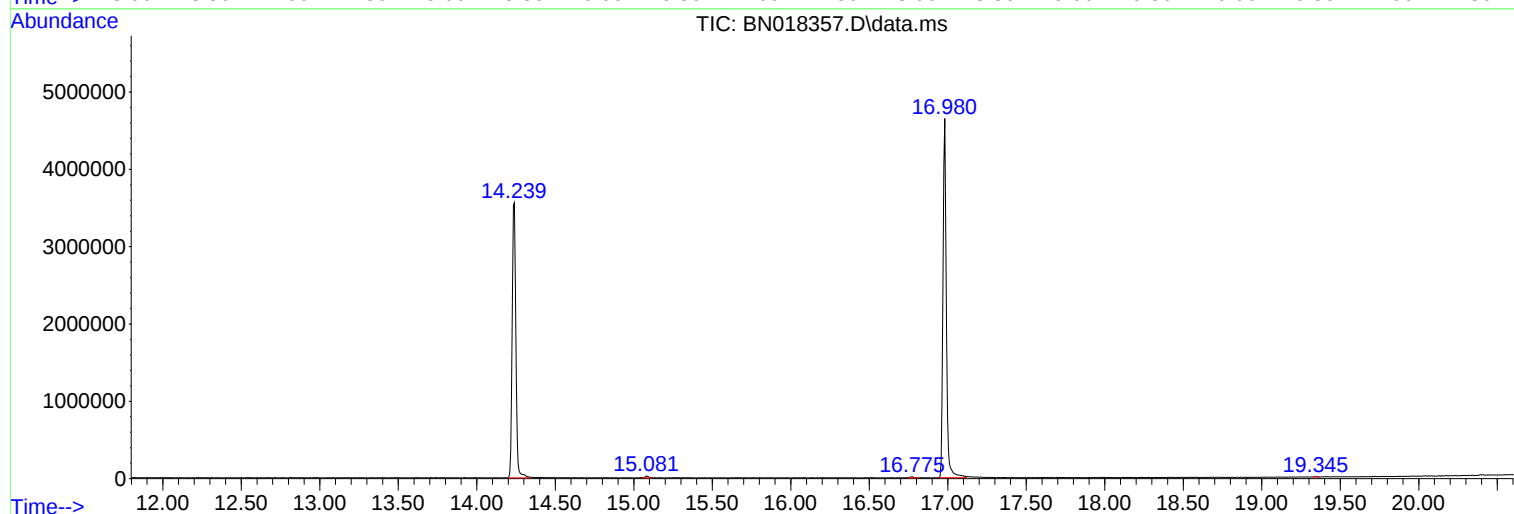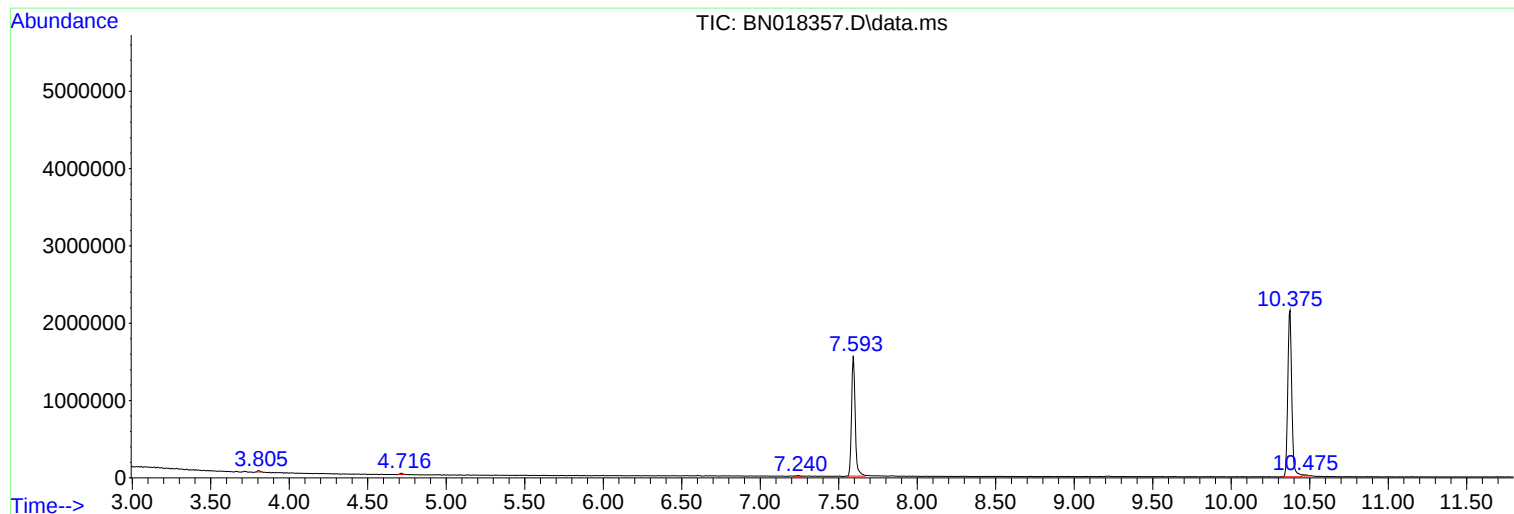

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018357.D
Acq On : 06 Jan 2022 18:06
Operator : CG/JU
Sample : N1026-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010622\
Data File : BN018357.D
Acq On : 06 Jan 2022 18:06
Operator : CG/JU
Sample : N1026-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BGLG9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc