
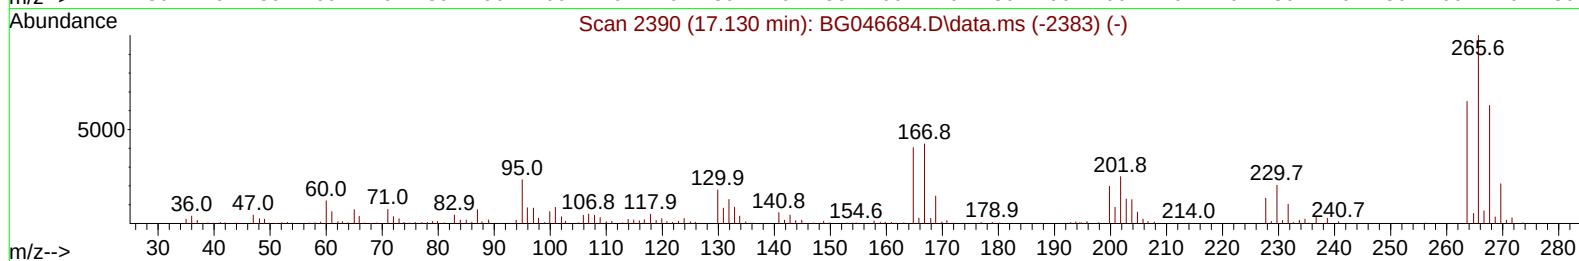
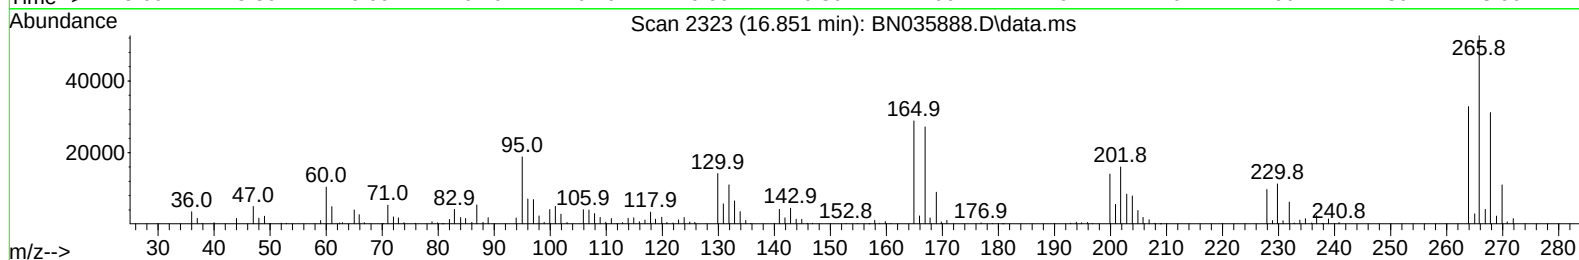


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN010625\  
Data File : BN035888.D  
Acq On : 06 Jan 2025 09:26  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 13:15:20 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 25 04:23:53 2024  
Response via : Initial Calibration

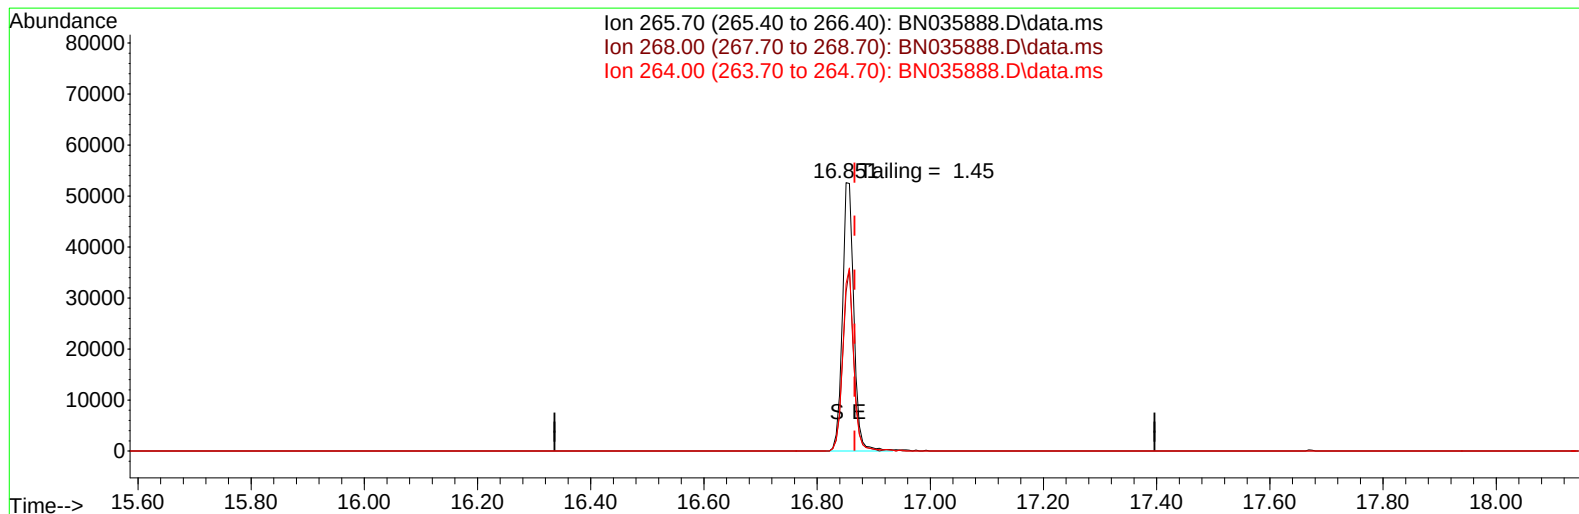

TIC: BN035888.D\data.ms

**(70) Pentachlorophenol (C)**




**16.851min (-0.015) 21827.15 ng**

**response 73999**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 62.20  | 59.23  |
| 264.00 | 61.60  | 62.38  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN010625\  
Data File : BN035888.D  
Acq On : 06 Jan 2025 09:26  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 06 13:15:20 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Dec 25 04:23:53 2024  
Response via : Initial Calibration

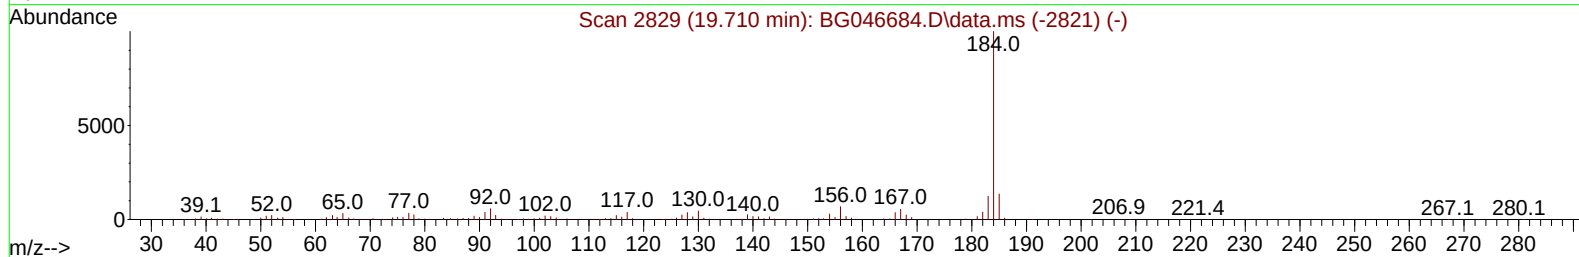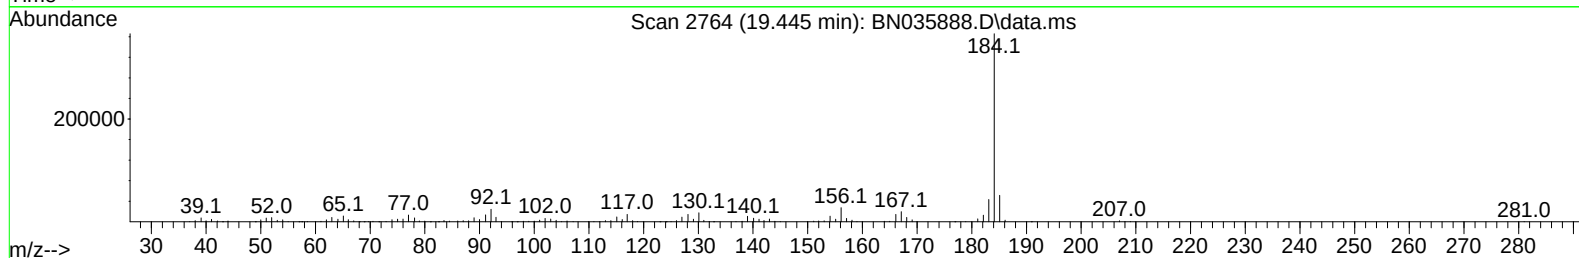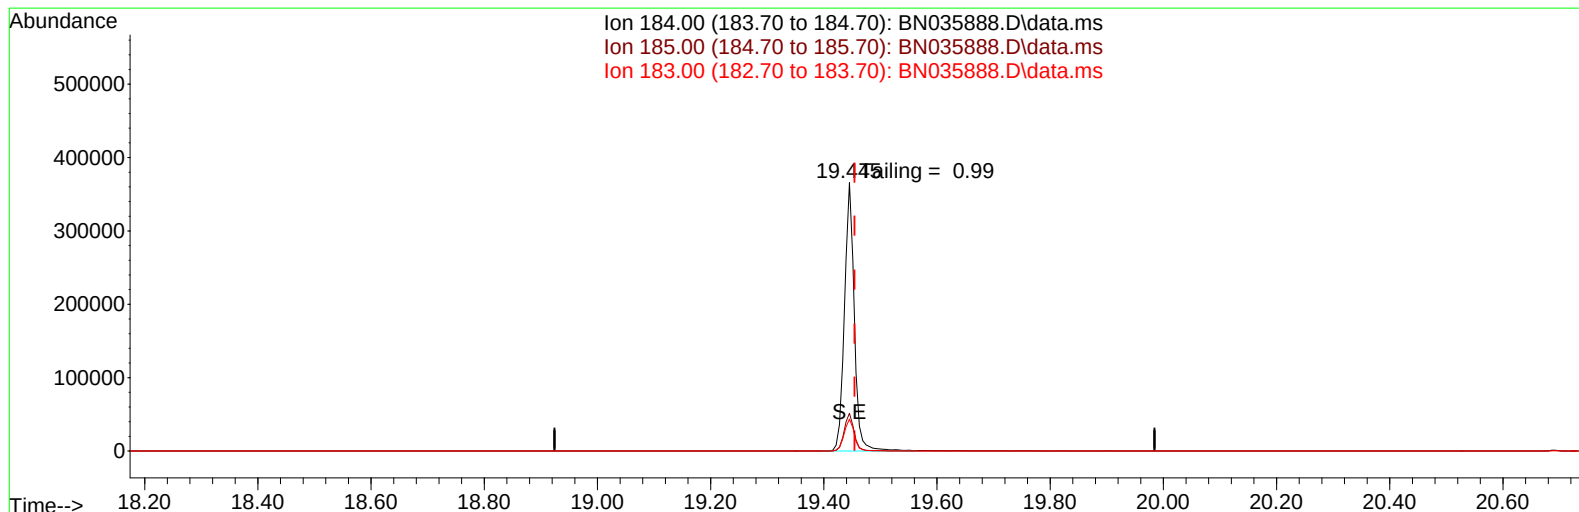

TIC: BN035888.D\data.ms

**(77) Benzidine**

19.445min (-0.009) 0.00 ng

response 444563

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 14.07  |
| 183.00 | 13.20  | 11.86  |
| 0.00   | 0.00   | 0.00   |