
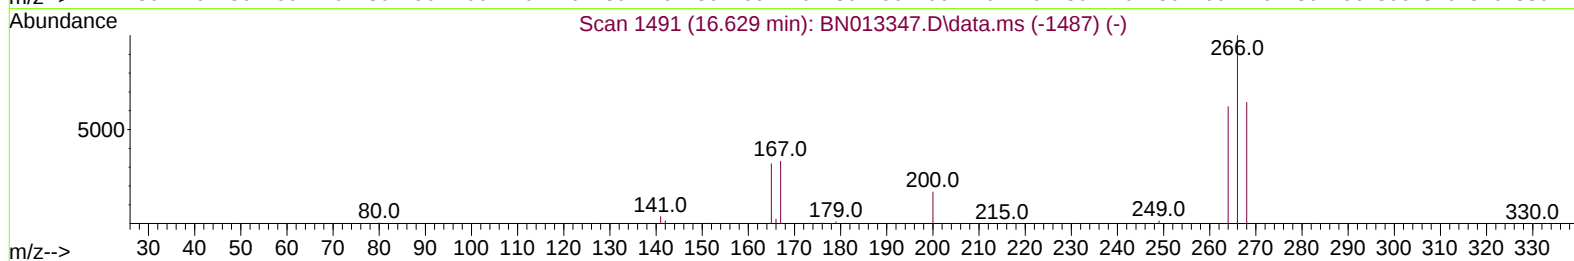
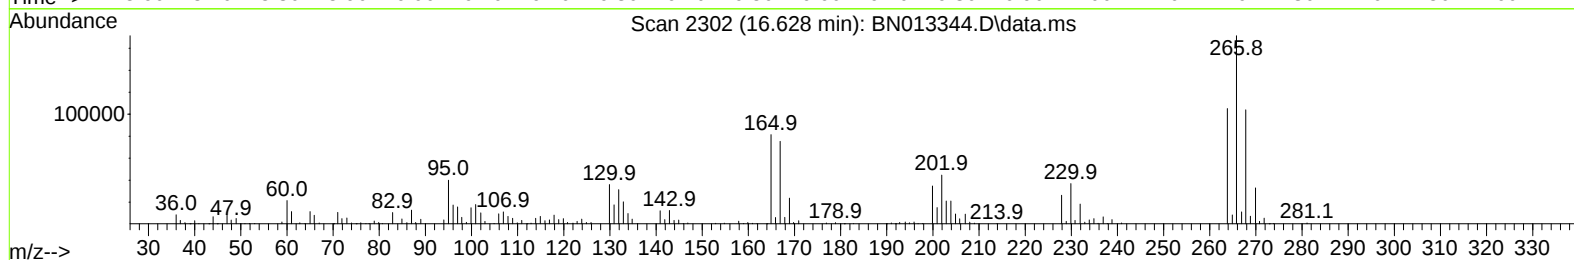


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010721\
 Data File : BN013344.D
 Acq On : 07 Jan 2021 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 08 03:38:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 07 16:27:07 2021
 Response via : Initial Calibration

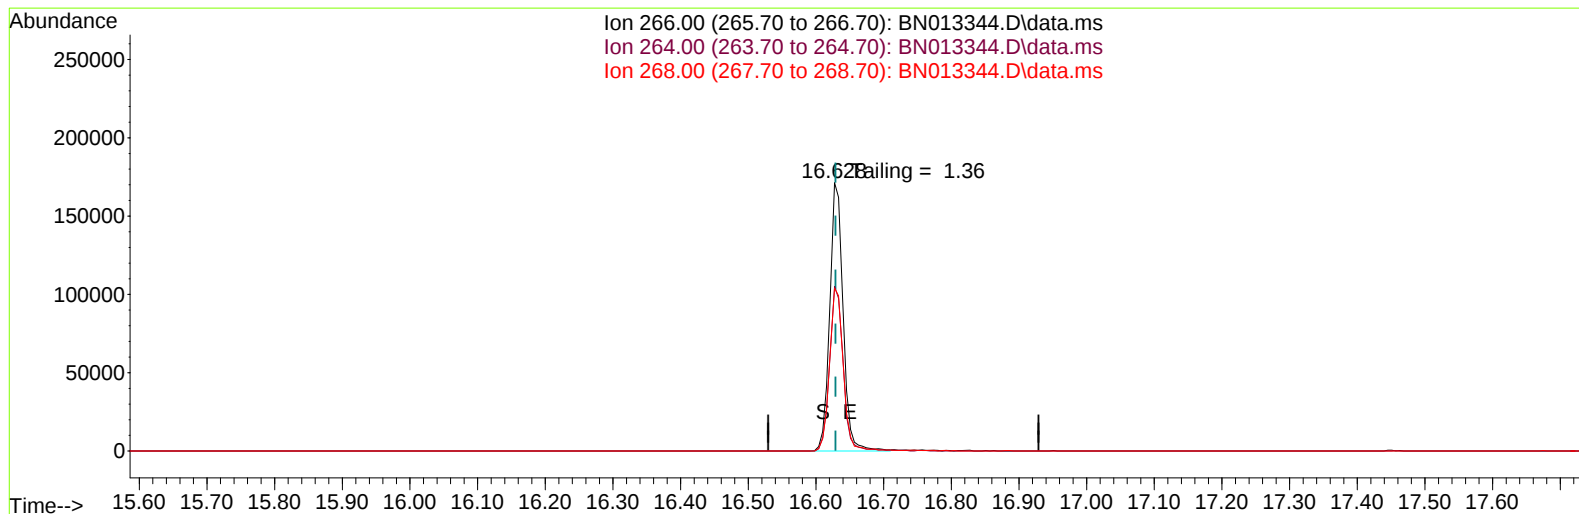

TIC: BN013344.D\data.ms

(24) Pentachlorophenol

16.628min (-0.002) 0.00 ng

response 235703

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	61.80
268.00	68.30	62.34
0.00	0.00	0.00