


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010721\
 Data File : BN013344.D
 Acq On : 07 Jan 2021 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 07 16:27:07 2021

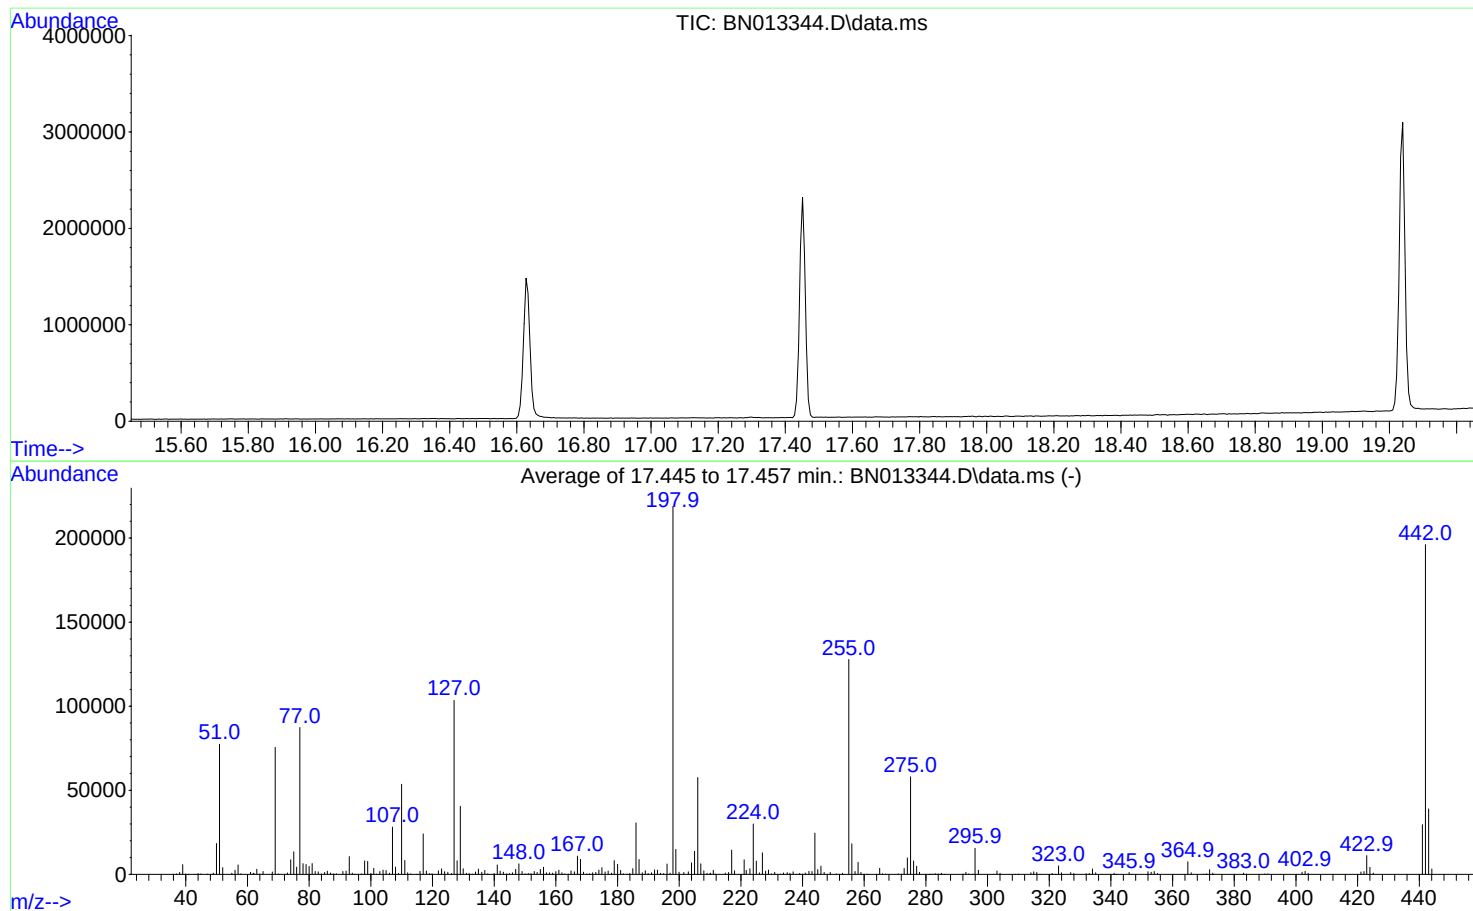

AutoFind: Scans 2441, 2442, 2443; Background Corrected with Scan 2435

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.4	77357	PASS
68	69	0.00	2	1.9	1471	PASS
69	198	0.00	100	34.5	75541	PASS
70	69	0.00	2	0.4	330	PASS
127	198	10	80	47.3	103464	PASS
197	198	0.00	2	0.4	808	PASS
198	198	100	100	100.0	218773	PASS
199	198	5	9	6.8	14866	PASS
275	198	10	60	26.6	58096	PASS
365	198	1	100	3.4	7508	PASS
441	198	0.01	100	13.5	29619	PASS
442	442	50	100	100.0	196117	PASS
443	442	15	24	19.9	38965	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/7/2021	BNA_N	<u>BN013344.D</u>
Compound Name	Response	Retention Time
DDT	755300	20.486
DDD	7760	20.045
DDE	1187	19.539
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8947	764247	1.17

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010721\
 Data File : BN013344.D
 Acq On : 07 Jan 2021 10:52
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Jan 08 03:38:23 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 07 16:27:07 2021
 Response via : Initial Calibration

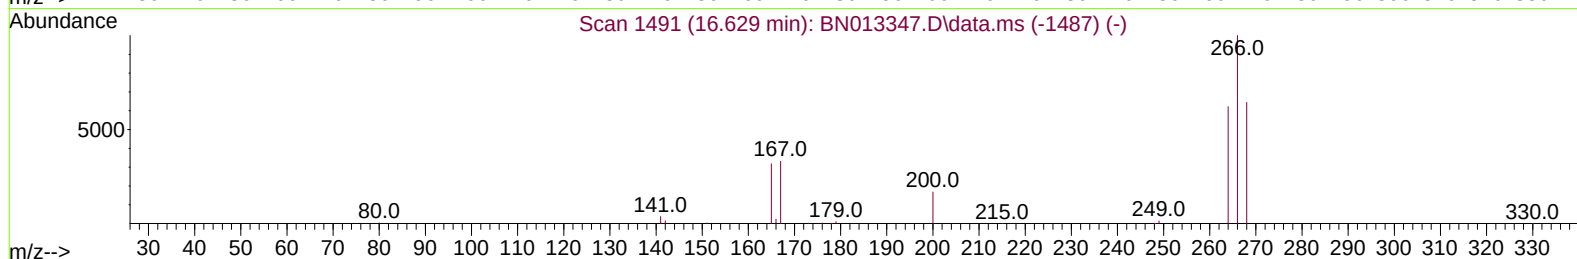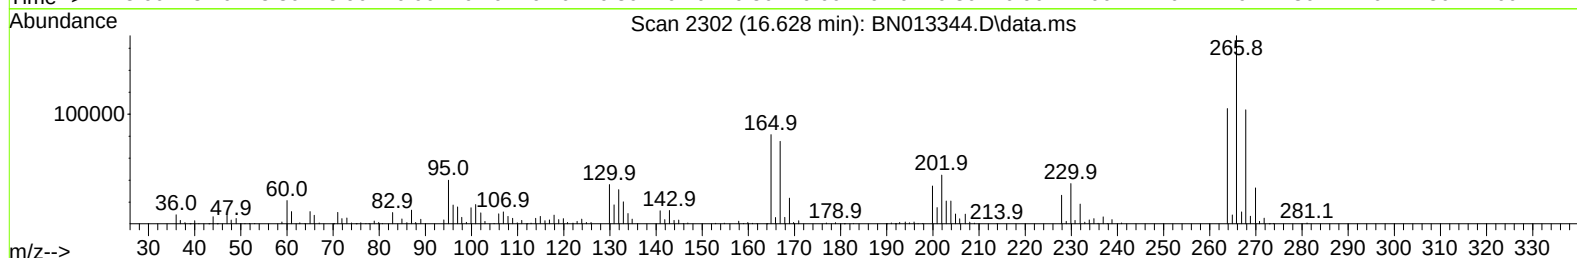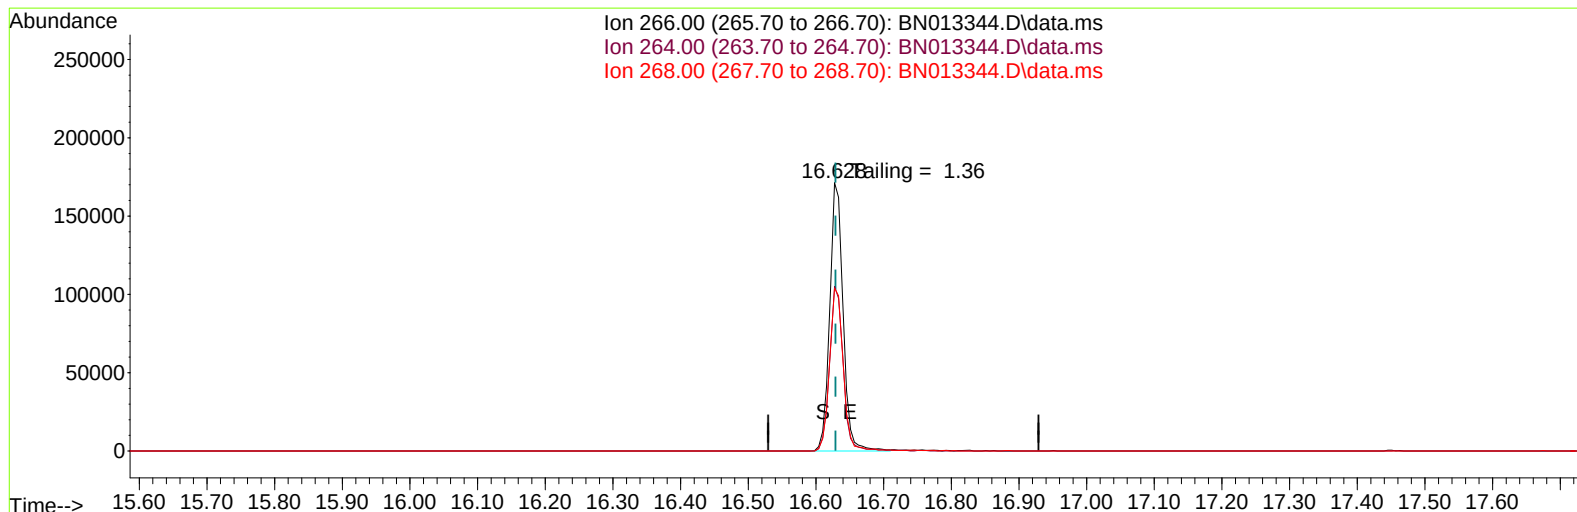

TIC: BN013344.D\data.ms

(24) Pentachlorophenol

16.628min (-0.002) 0.00 ng

response 235703

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.50	61.80
268.00	68.30	62.34
0.00	0.00	0.00