


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010725\
Data File : BN035896.D
Acq On : 07 Jan 2025 14:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

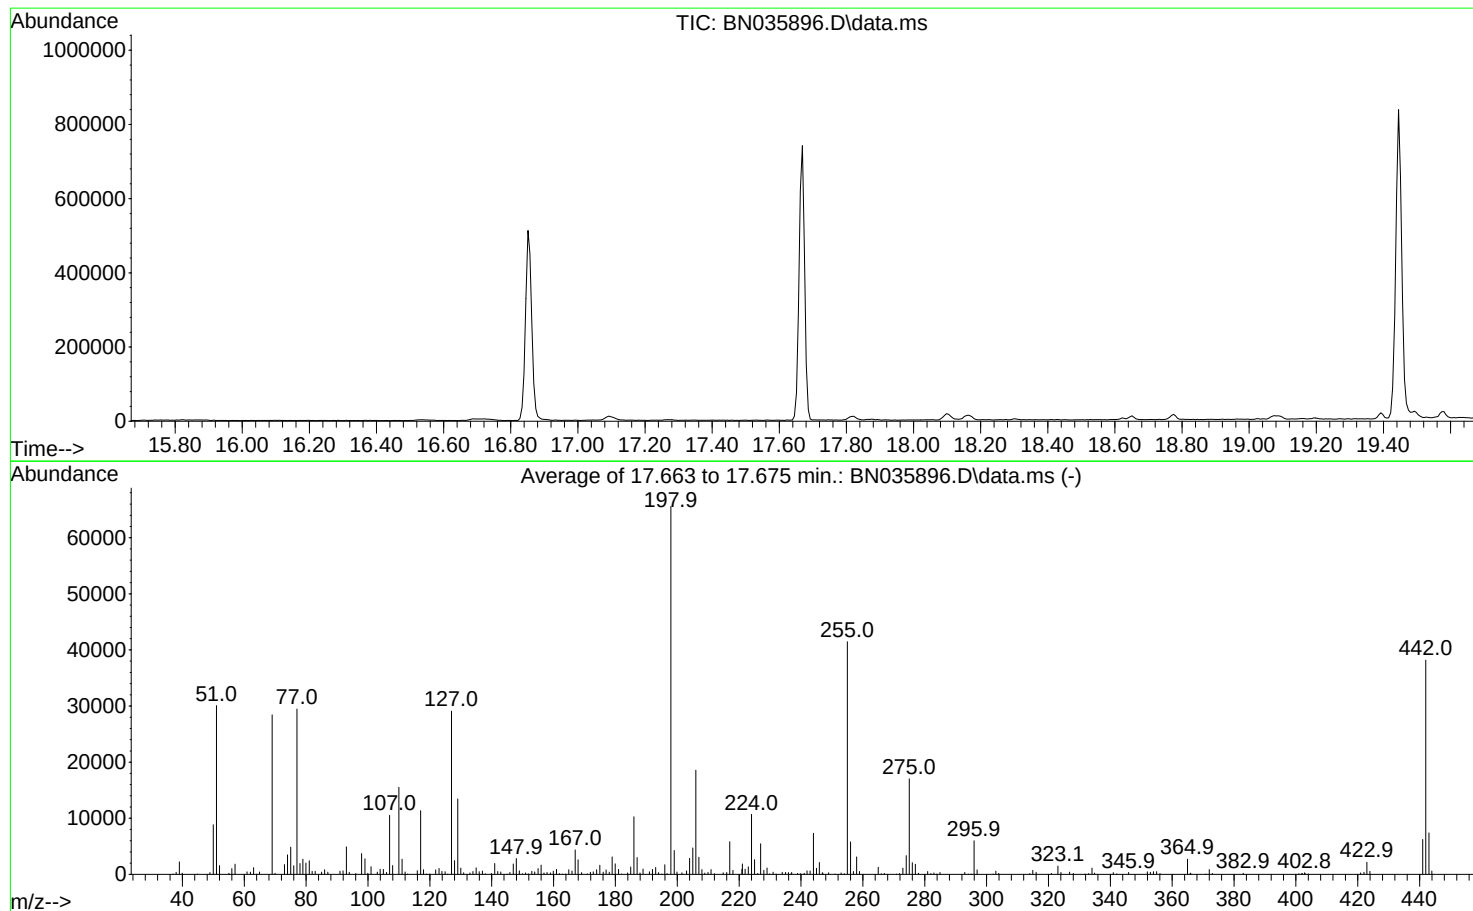

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	30080	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.4	28445	PASS
70	69	0.00	2	0.7	197	PASS
127	198	10	80	44.4	29099	PASS
197	198	0.00	2	0.2	155	PASS
198	198	100	100	100.0	65563	PASS
199	198	5	9	6.5	4240	PASS
275	198	10	60	26.0	17034	PASS
365	198	1	100	4.1	2710	PASS
441	198	0.01	100	9.5	6208	PASS
442	442	50	100	100.0	38176	PASS
443	442	15	24	19.4	7393	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/7/2025	BNA_N	<u>BN035896.D</u>
Compound Name	Response	Retention Time
DDT	189369	20.692
DDD	3147	20.304
DDE	77	19.745
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3224	192593	1.67

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010725\
Data File : BN035896.D
Acq On : 07 Jan 2025 14:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 07 18:12:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

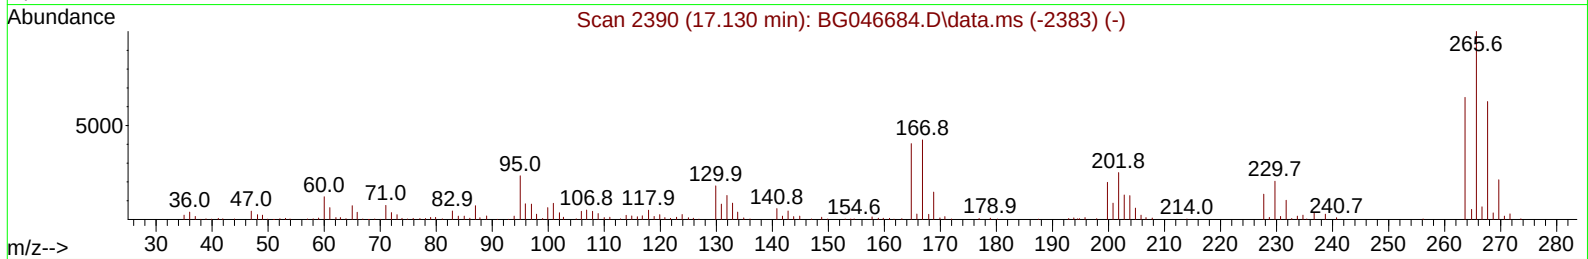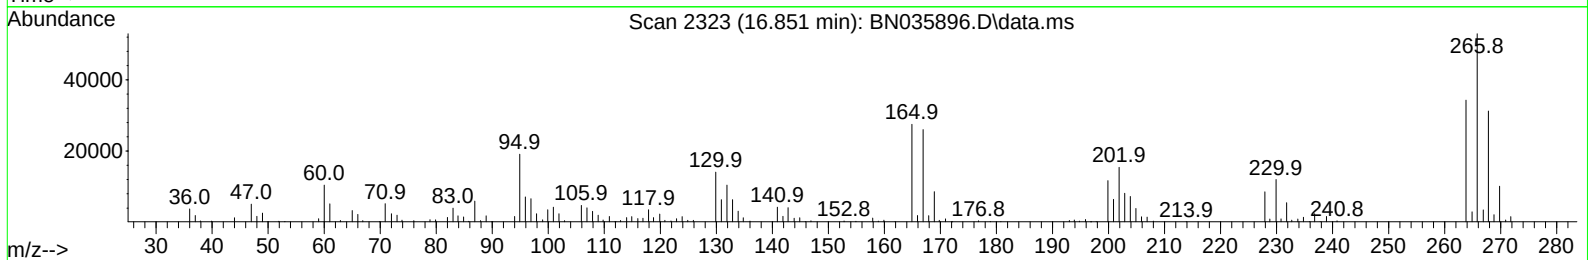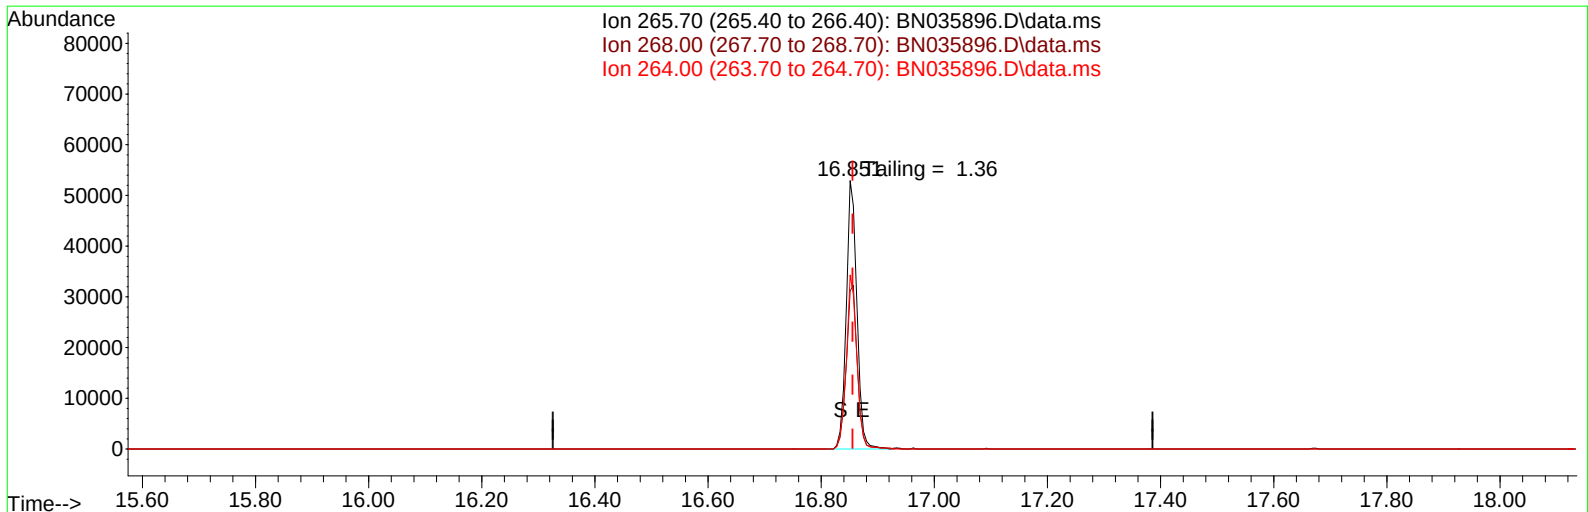

TIC: BN035896.D\data.ms

(70) Pentachlorophenol (C)

16.851min (-0.005) 25946.00 ng m




response 69230

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.99
264.00	61.60	64.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN010725\
Data File : BN035896.D
Acq On : 07 Jan 2025 14:24
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 07 18:12:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

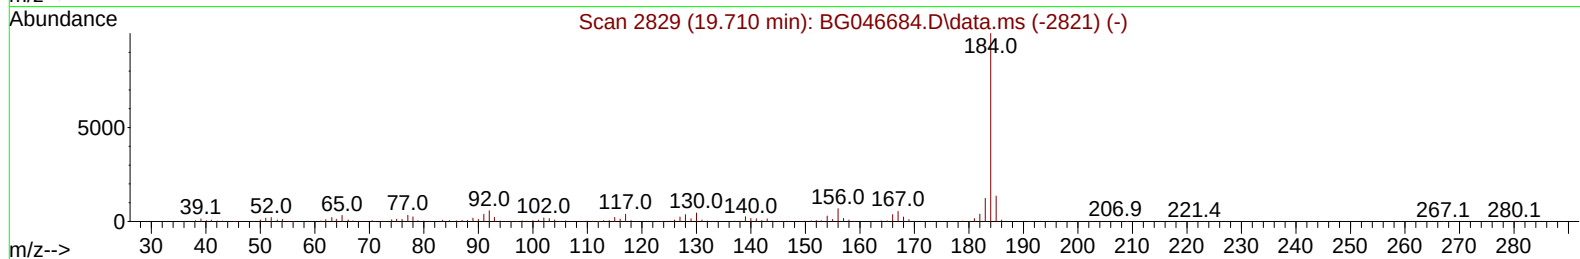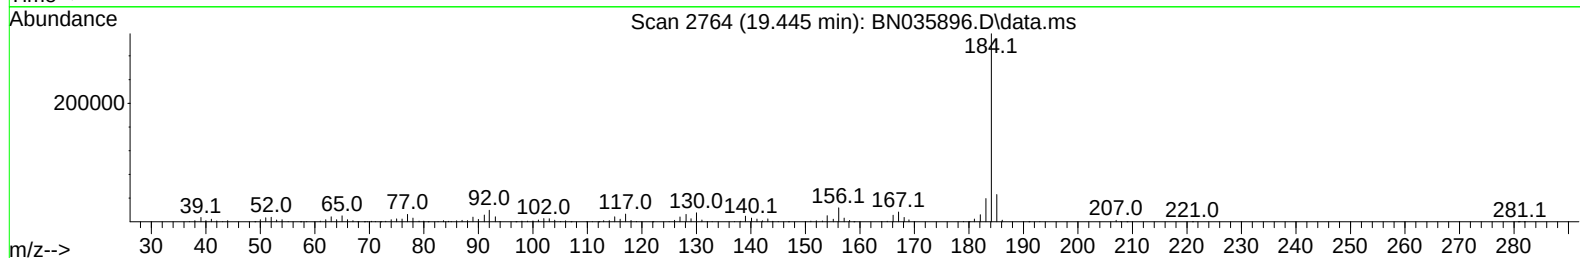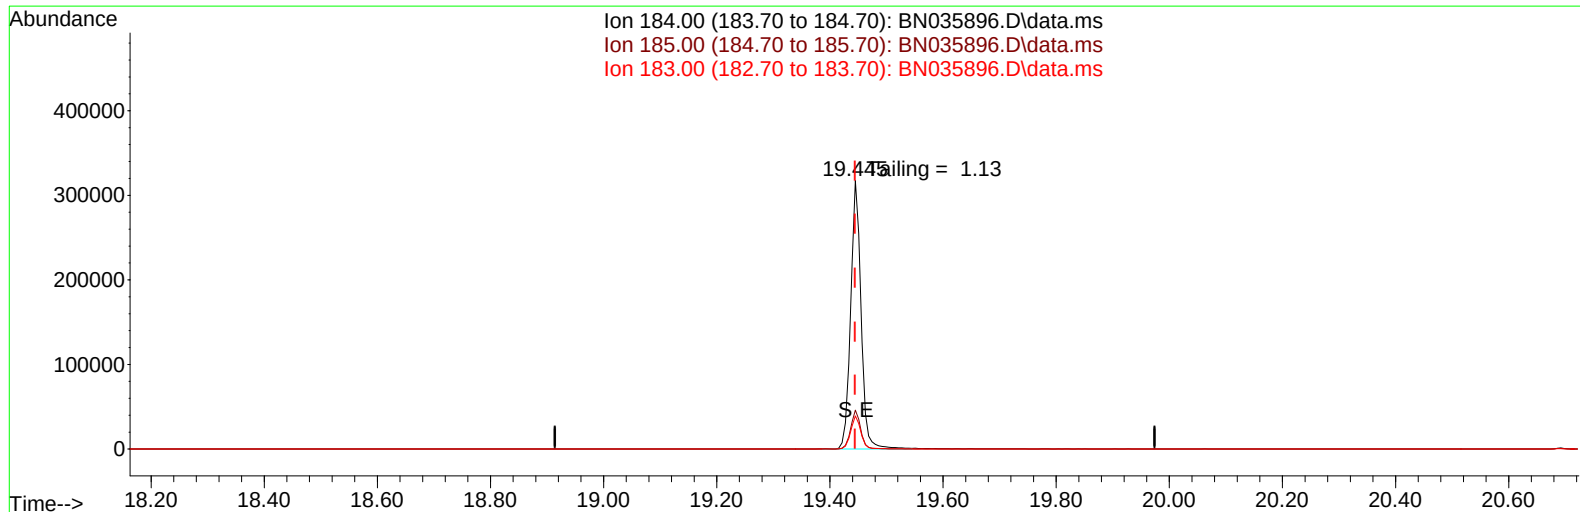

TIC: BN035896.D\data.ms

(77) Benzidine

19.445min (+ 0.001) 0.00 ng

response 408901

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.53
183.00	13.20	12.37
0.00	0.00	0.00