
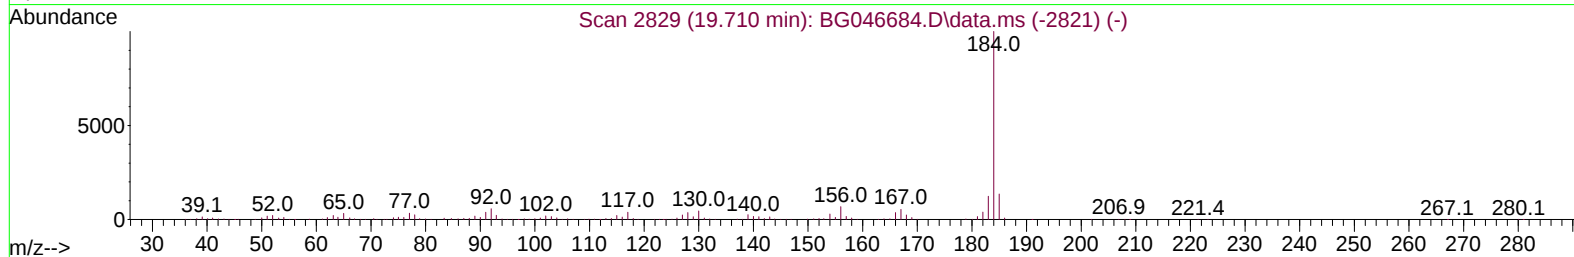
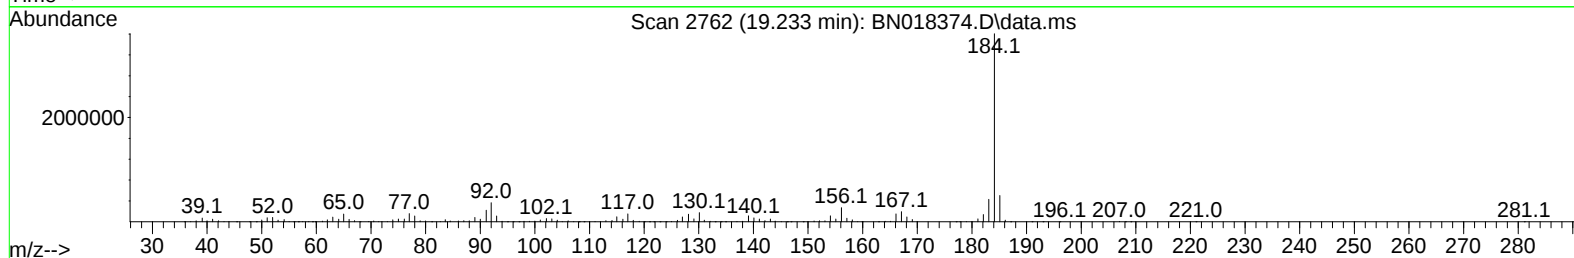


Data Path : Z:\svoasrv\HPCHEM1\BNA\_N\Data\BN011022\  
 Data File : BN018374.D  
 Acq On : 10 Jan 2022 10:00  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 14:39:47 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_N\Methods\8270E-Tune.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Jan 10 14:39:41 2022  
 Response via : Initial Calibration

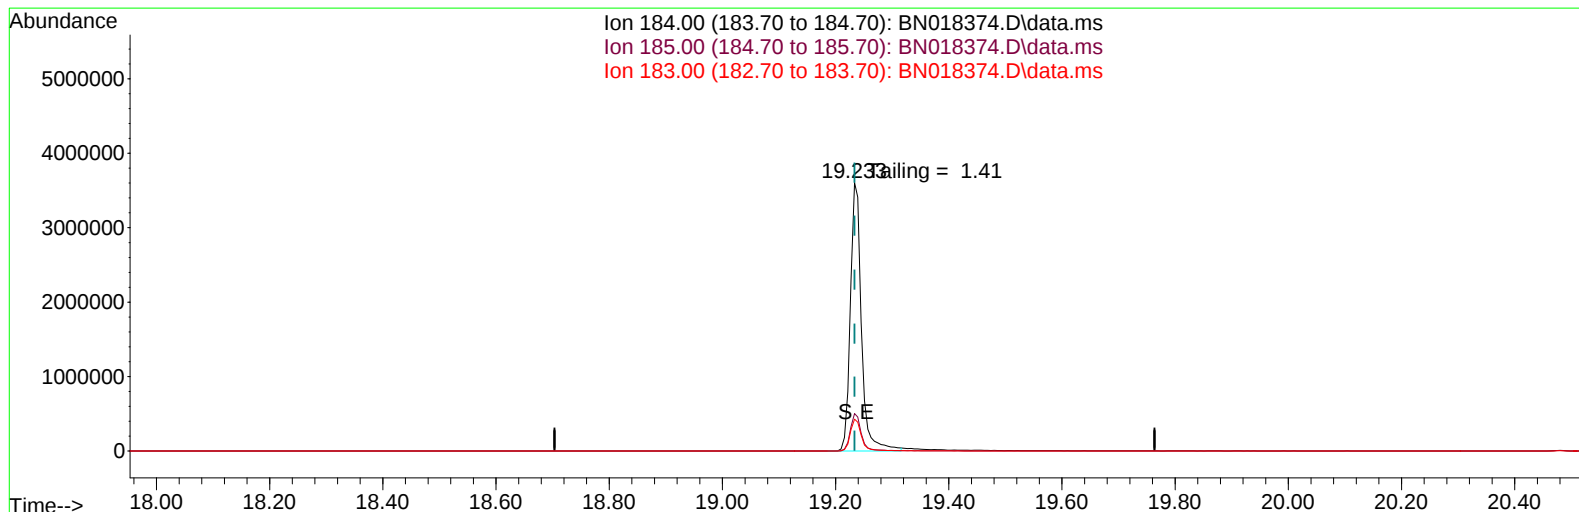

TIC: BN018374.D\data.ms

**(77) Benzidine**

19.233min ( 0.000) 0.00 ng

response 5017382

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.50  | 13.96  |
| 183.00 | 13.20  | 11.89  |
| 0.00   | 0.00   | 0.00   |