
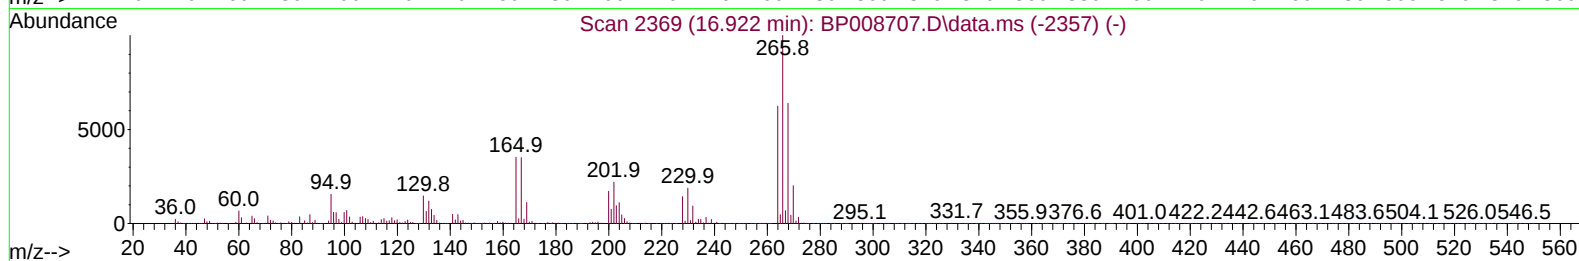
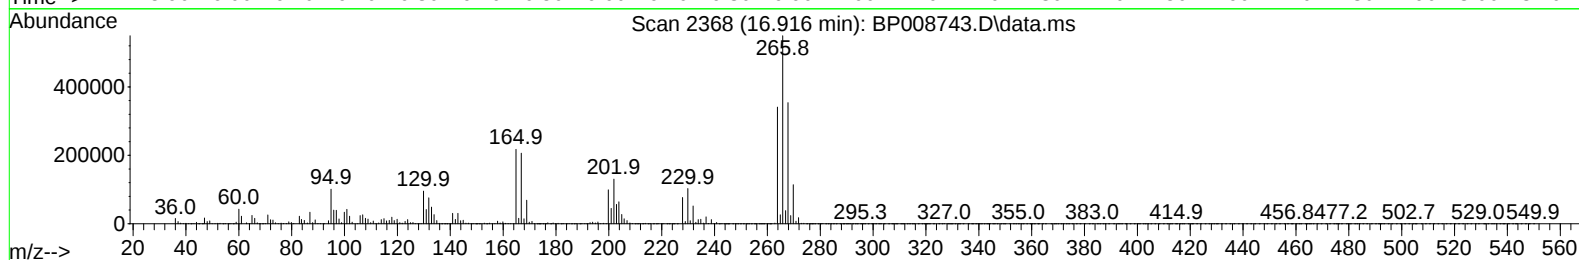


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP011022\  
 Data File : BP008743.D  
 Acq On : 10 Jan 2022 10:17  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 16:49:21 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP010622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Fri Jan 07 07:45:52 2022  
 Response via : Initial Calibration

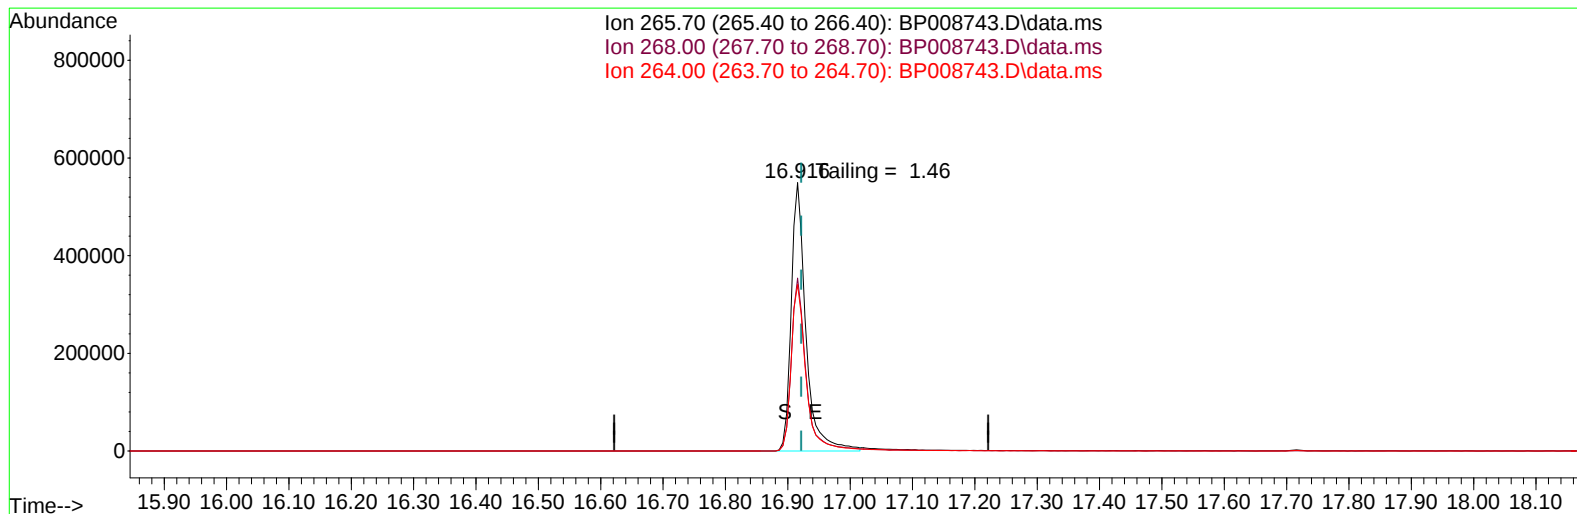

TIC: BP008743.D\data.ms

**(70) Pentachlorophenol (C)**

16.916min (-0.006) 176016.36 ng

response 927250

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.60  | 64.45  |
| 264.00 | 62.90  | 62.03  |
| 0.00   | 0.00   | 0.00   |