
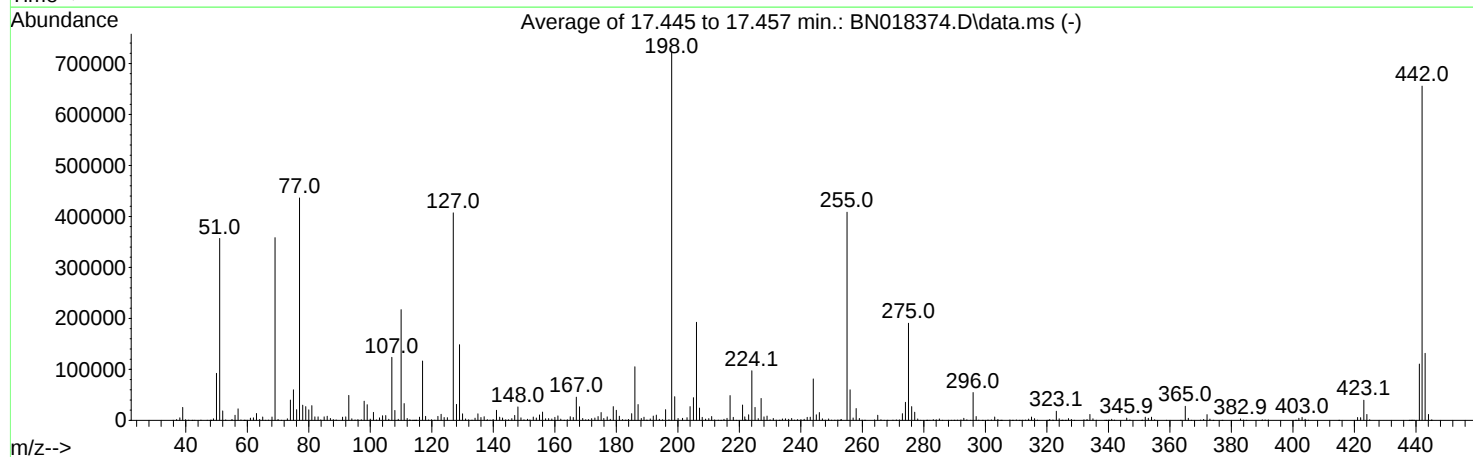


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011022\
 Data File : BN018374.D
 Acq On : 10 Jan 2022 10:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 10 13:58:28 2022

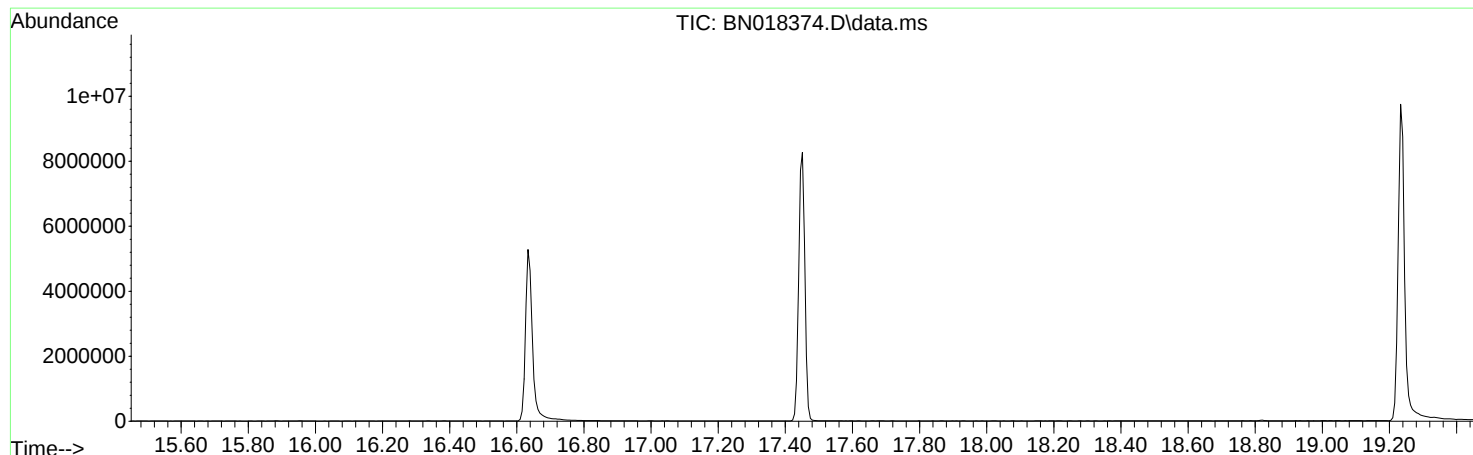

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2451

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.4	356757	PASS
68	69	0.00	2	1.8	6526	PASS
69	198	0.00	100	49.7	358336	PASS
70	69	0.00	2	0.5	1874	PASS
127	198	10	80	56.4	406955	PASS
197	198	0.00	2	0.2	1209	PASS
198	198	100	100	100.0	721579	PASS
199	198	5	9	6.5	46589	PASS
275	198	10	60	26.4	190549	PASS
365	198	1	100	3.9	27795	PASS
441	198	0.01	100	15.3	110429	PASS
442	442	50	100	100.0	655552	PASS
443	442	15	24	20.0	131435	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/10/2022	BNA_N	<u>BN018374.D</u>
Compound Name	Response	Retention Time
DDT	2406853	20.48
DDD	7804	20.03
DDE	788	19.52
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8592	2415445	0.36

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011022\
Data File : BN018374.D
Acq On : 10 Jan 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 10 14:39:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 10 14:39:41 2022
Response via : Initial Calibration

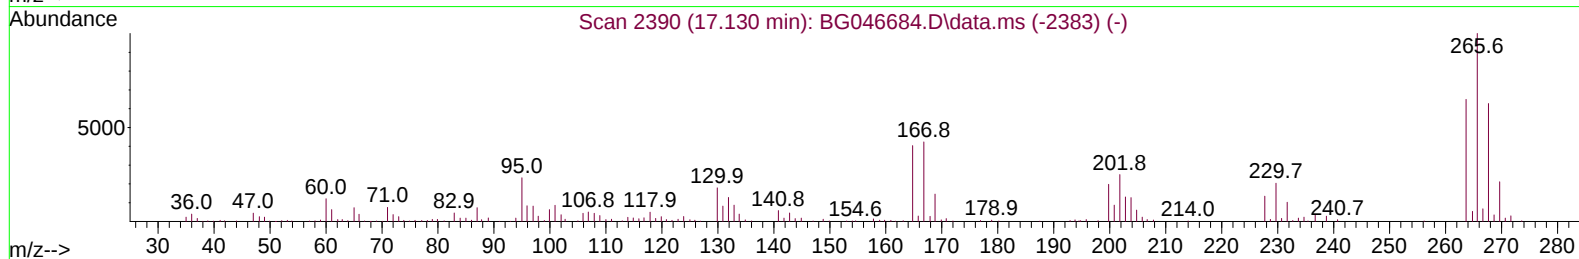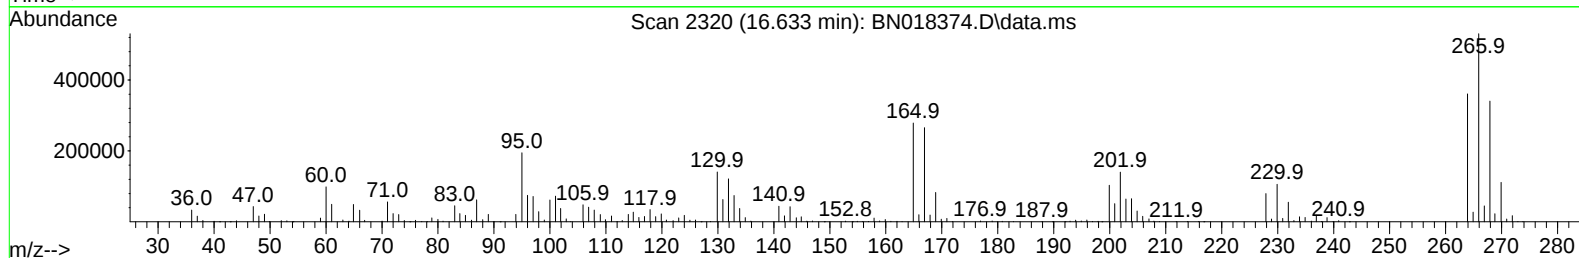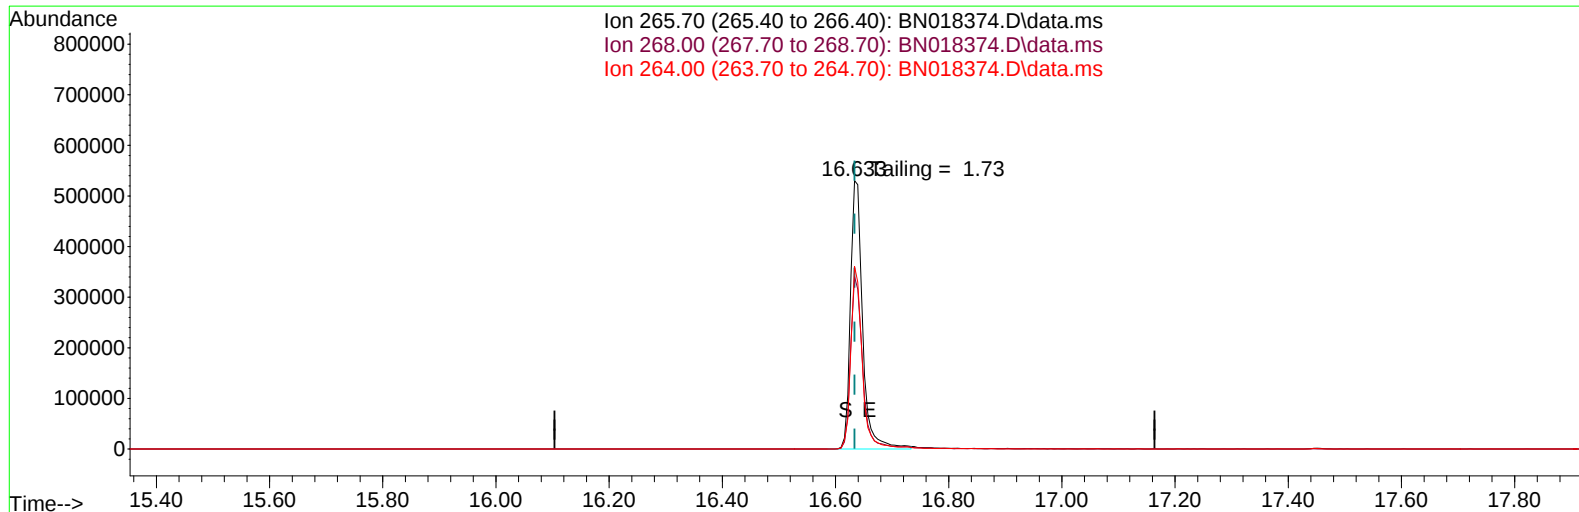

TIC: BN018374.D\data.ms

(70) Pentachlorophenol (C)

16.633min (0.000) 18542.93 ng




response 805018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.22
264.00	61.60	68.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011022\
Data File : BN018374.D
Acq On : 10 Jan 2022 10:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 10 14:39:47 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 10 14:39:41 2022
Response via : Initial Calibration

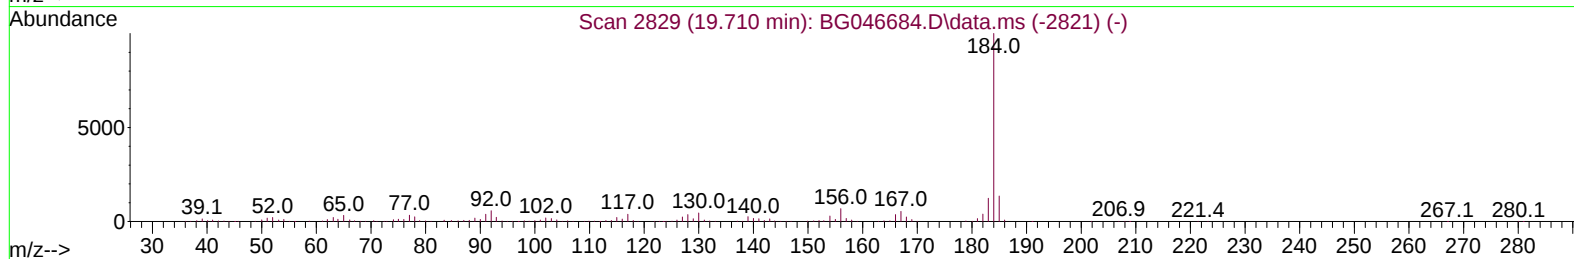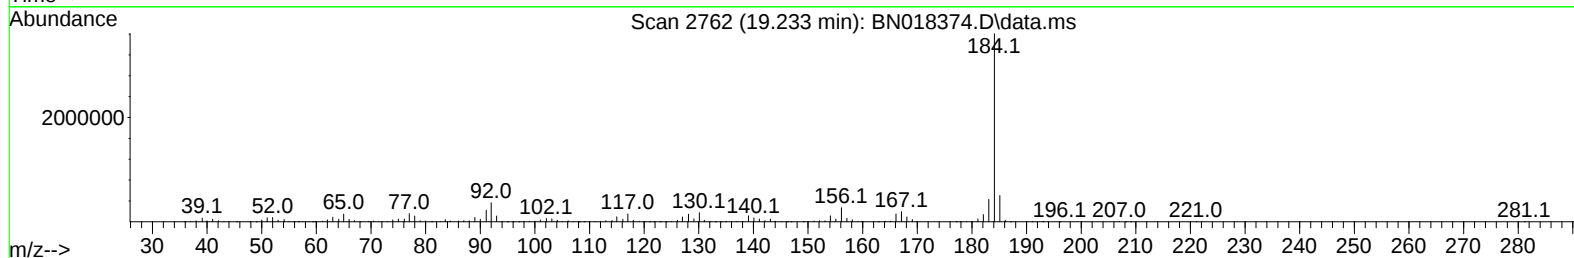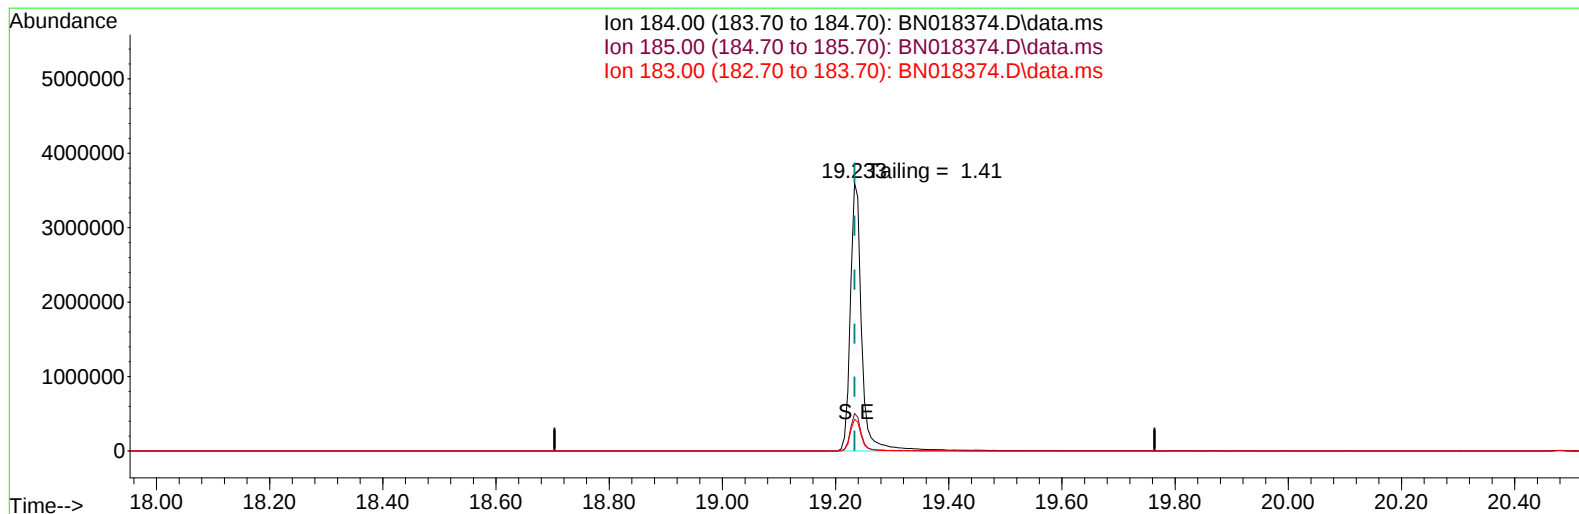

TIC: BN018374.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 5017382

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.96
183.00	13.20	11.89
0.00	0.00	0.00