

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011122\
 Data File : BN018382.D
 Acq On : 11 Jan 2022 11:11
 Operator : CG/JU
 Sample : PB141950BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK950

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018382.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	22	rVB	130522	175986	1.50%	0.133%
2	3.458	77	80	99	rBV	1892381	2853051	24.29%	2.164%
3	3.793	134	137	148	rVB3	37245	63459	0.54%	0.048%
4	6.769	637	643	661	rBV	2356888	3693588	31.45%	2.801%
5	6.922	663	669	686	rVB	1865735	3026754	25.77%	2.296%
6	7.122	696	703	715	rBV	2352882	3733680	31.79%	2.832%
7	7.587	775	782	789	rBV	1826909	2886371	24.57%	2.189%
8	8.304	897	904	922	rBV	2714669	4462205	37.99%	3.384%
9	8.734	969	977	988	rBV	2245600	3542999	30.16%	2.687%
10	9.457	1092	1100	1109	rBV	1827877	3036952	25.86%	2.303%
11	9.993	1184	1191	1205	rBV	2530628	4342041	36.97%	3.293%
12	10.363	1247	1254	1267	rBV	2614316	4290487	36.53%	3.254%
13	10.504	1271	1278	1299	rBV	2599159	4652193	39.61%	3.528%
14	11.975	1522	1528	1536	rBV2	31063	67571	0.58%	0.051%
15	13.210	1733	1738	1740	rBV5	8841	13460	0.11%	0.010%
16	13.651	1807	1813	1822	rBV	4905876	6669919	56.78%	5.059%
17	13.922	1852	1859	1877	rBV	5501788	7976958	67.91%	6.050%
18	14.234	1905	1912	1920	rBV	3859562	5558925	47.33%	4.216%
19	14.445	1942	1948	1974	rBV	1640288	2979001	25.36%	2.259%
20	15.228	2072	2081	2093	rBV	6591362	9451836	80.47%	7.168%
21	15.357	2097	2103	2115	rVV	2133494	3053578	26.00%	2.316%
22	15.469	2118	2122	2132	rVB3	38086	72789	0.62%	0.055%
23	16.016	2210	2215	2220	rVB7	6617	12275	0.10%	0.009%
24	16.657	2320	2324	2328	rBV5	7105	12335	0.11%	0.009%
25	16.763	2336	2342	2346	rBV3	19565	29784	0.25%	0.023%
26	16.975	2372	2378	2388	rBV	4571043	6395850	54.45%	4.851%
27	17.075	2389	2395	2407	rVV2	7377263	10300847	87.70%	7.812%
28	17.663	2486	2495	2501	rVB7	11548	20294	0.17%	0.015%
29	17.898	2531	2535	2541	rBV5	27724	60372	0.51%	0.046%
30	18.198	2582	2586	2589	rBV5	12056	17694	0.15%	0.013%
31	18.939	2707	2712	2717	rBV3	85682	114632	0.98%	0.087%
32	19.010	2719	2724	2731	rVV2	82778	118657	1.01%	0.090%
33	19.192	2752	2755	2759	rBV6	14770	22637	0.19%	0.017%
34	19.375	2778	2786	2797	rBV	8671193	11745946	100.00%	8.908%
35	20.451	2966	2969	2973	rBV5	18786	27471	0.23%	0.021%
36	20.692	3007	3010	3015	rVB7	34951	37153	0.32%	0.028%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011122\
Data File : BN018382.D
Acq On : 11 Jan 2022 11:11
Operator : CG/JU
Sample : PB141950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Title : SVOA CALIBRATION

37	20.763	3019	3022	3027	rBV4	41633	53860	0.46%	0.041%
38	21.010	3061	3064	3071	rBV8	33850	58085	0.49%	0.044%
39	21.174	3086	3092	3107	rBV	5212264	6661228	56.71%	5.052%
40	21.357	3120	3123	3125	rBV4	33075	33823	0.29%	0.026%
41	21.780	3192	3195	3198	rBV3	45618	56581	0.48%	0.043%
42	22.245	3270	3274	3281	rVB2	76775	117561	1.00%	0.089%
43	22.751	3356	3360	3364	rBV2	103380	152954	1.30%	0.116%
44	23.251	3437	3445	3453	rBV	6300815	11683877	99.47%	8.861%
45	23.392	3462	3469	3485	rVB2	3644375	6989555	59.51%	5.301%
46	23.968	3562	3567	3575	rVB	145475	293217	2.50%	0.222%
47	24.727	3691	3696	3703	rVB	117979	234990	2.00%	0.178%




Sum of corrected areas: 131855481

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011122\
Data File : BN018382.D
Acq On : 11 Jan 2022 11:11
Operator : CG/JU
Sample : PB141950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

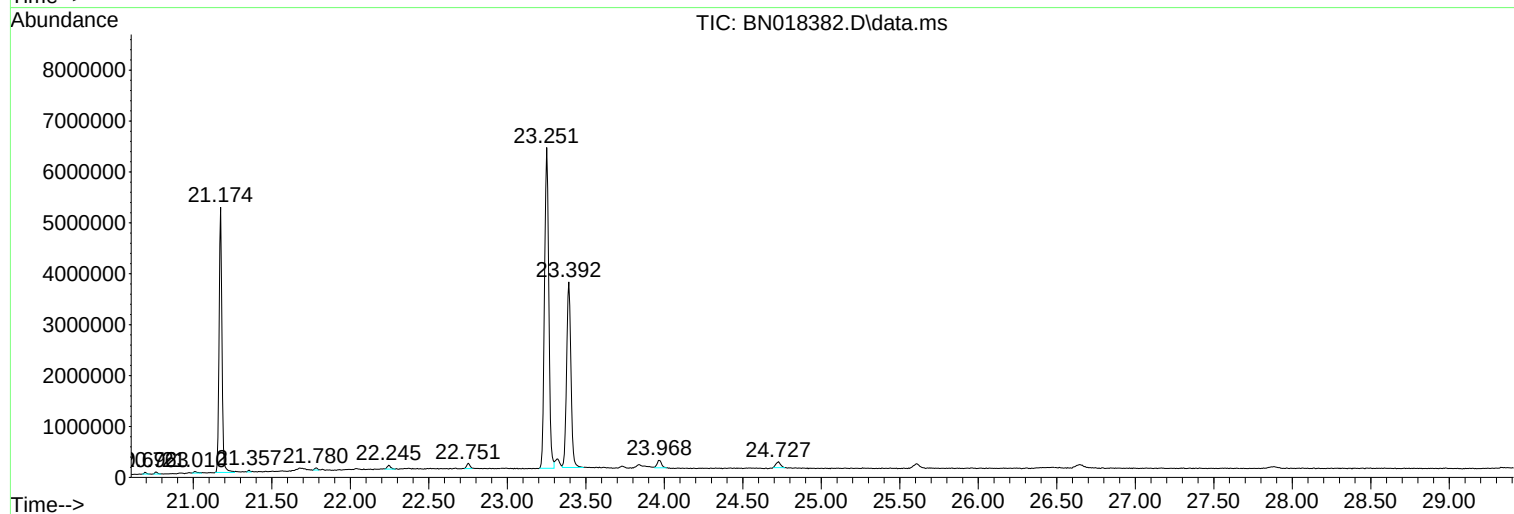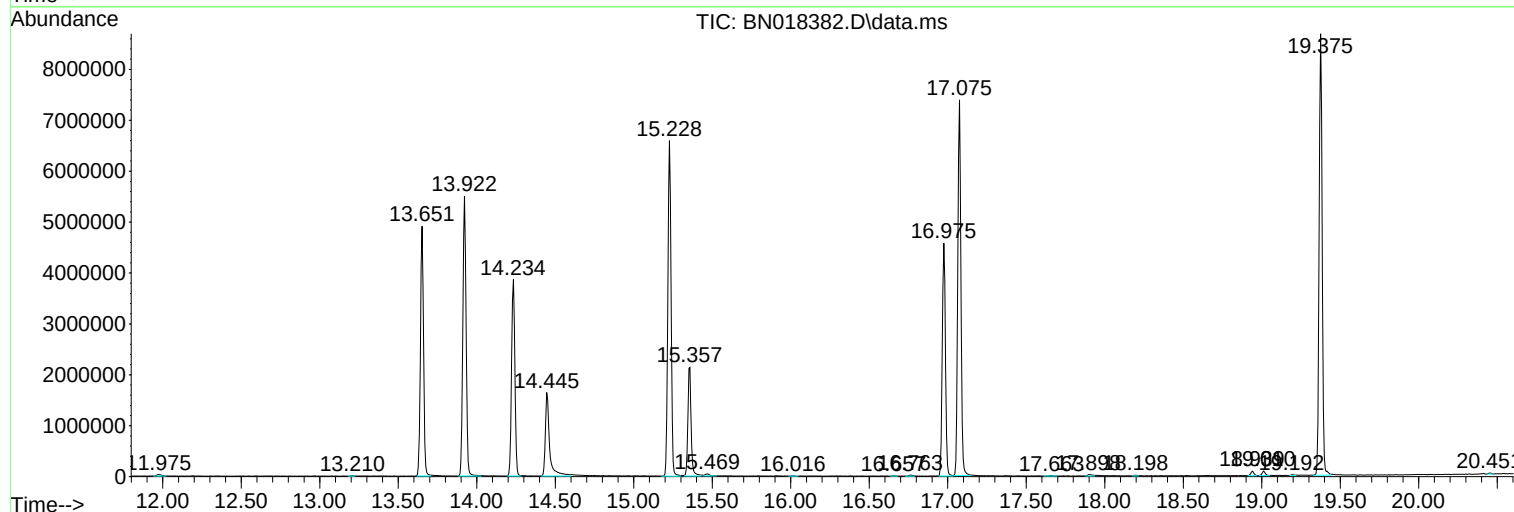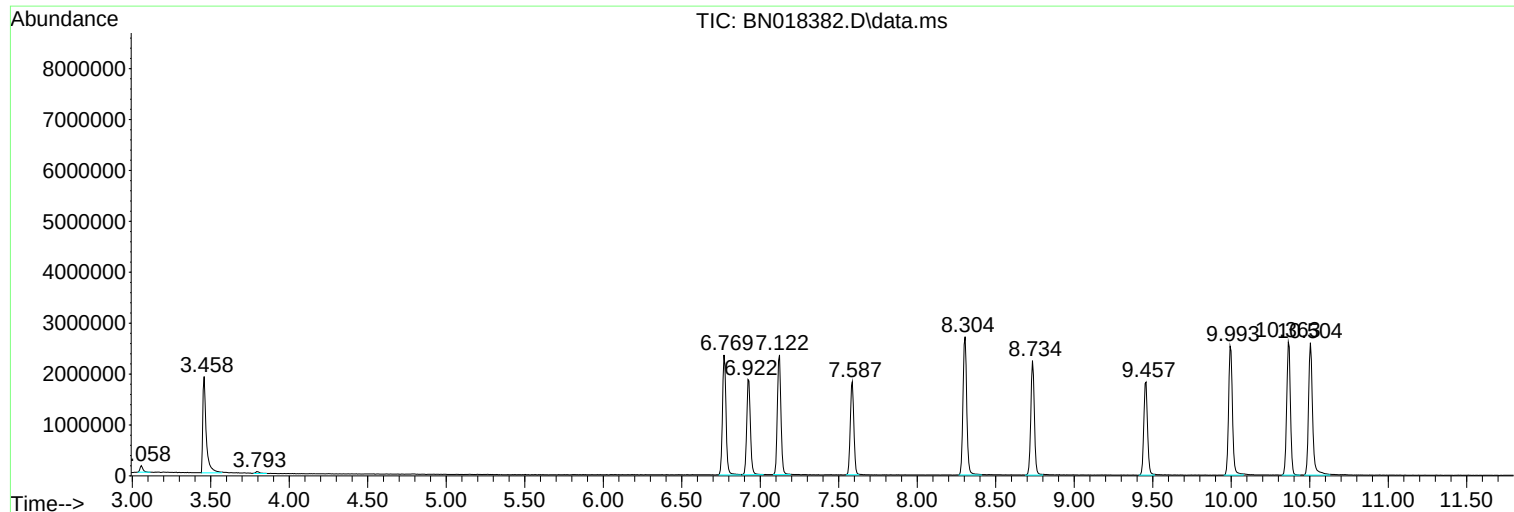

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011122\
Data File : BN018382.D
Acq On : 11 Jan 2022 11:11
Operator : CG/JU
Sample : PB141950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011122\
Data File : BN018382.D
Acq On : 11 Jan 2022 11:11
Operator : CG/JU
Sample : PB141950BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK950

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
