

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
 Data File : BN023613.D
 Acq On : 11 Jan 2023 15:53
 Operator : CG/JU
 Sample : 01050-04DL 30X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4477DL

Quant Time: Jan 11 16:28:21 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.946	152	111975	20.000	ng/u1	0.00
20) Naphthalene-d8	10.757	136	530991	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.598	164	330029	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	724805	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	635946	20.000	ng/u1	-0.01
88) Perylene-d12	23.957	264	683272	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.105	99	10332	1.041	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.275	67	8267	1.358	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	8307	1.093	ng/u1	0.00
15) 4-Methylphenol-d8	8.657	113	7586	0.958	ng/u1	-0.01
21) Nitrobenzene-d5	9.110	128	3895	0.973	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.840	143	3142	0.741	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.381	165	6434	0.796	ng/u1	0.00
31) 4-Chloroaniline-d4	10.910	131	11704	0.920	ng/u1	0.00
46) Dimethylphthalate-d6	14.010	166	26990	1.099	ng/u1	0.00
49) Acenaphthylene-d8	14.292	160	25936	0.953	ng/u1	0.00
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.587	176	24902	1.187	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.710	200	1819	0.416	ng/u1	0.00
73) Anthracene-d10	17.439	188	35291	1.088	ng/u1	-0.01
81) Pyrene-d10	19.739	212	42614	1.172	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.798	264	35955	1.064	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.445	149	3883985	150.378	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023613.D
Acq On : 11 Jan 2023 15:53
Operator : CG/JU
Sample : 01050-04DL 30X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4477DL

Quant Time: Jan 11 16:28:21 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 05 03:34:47 2023
Response via : Initial Calibration

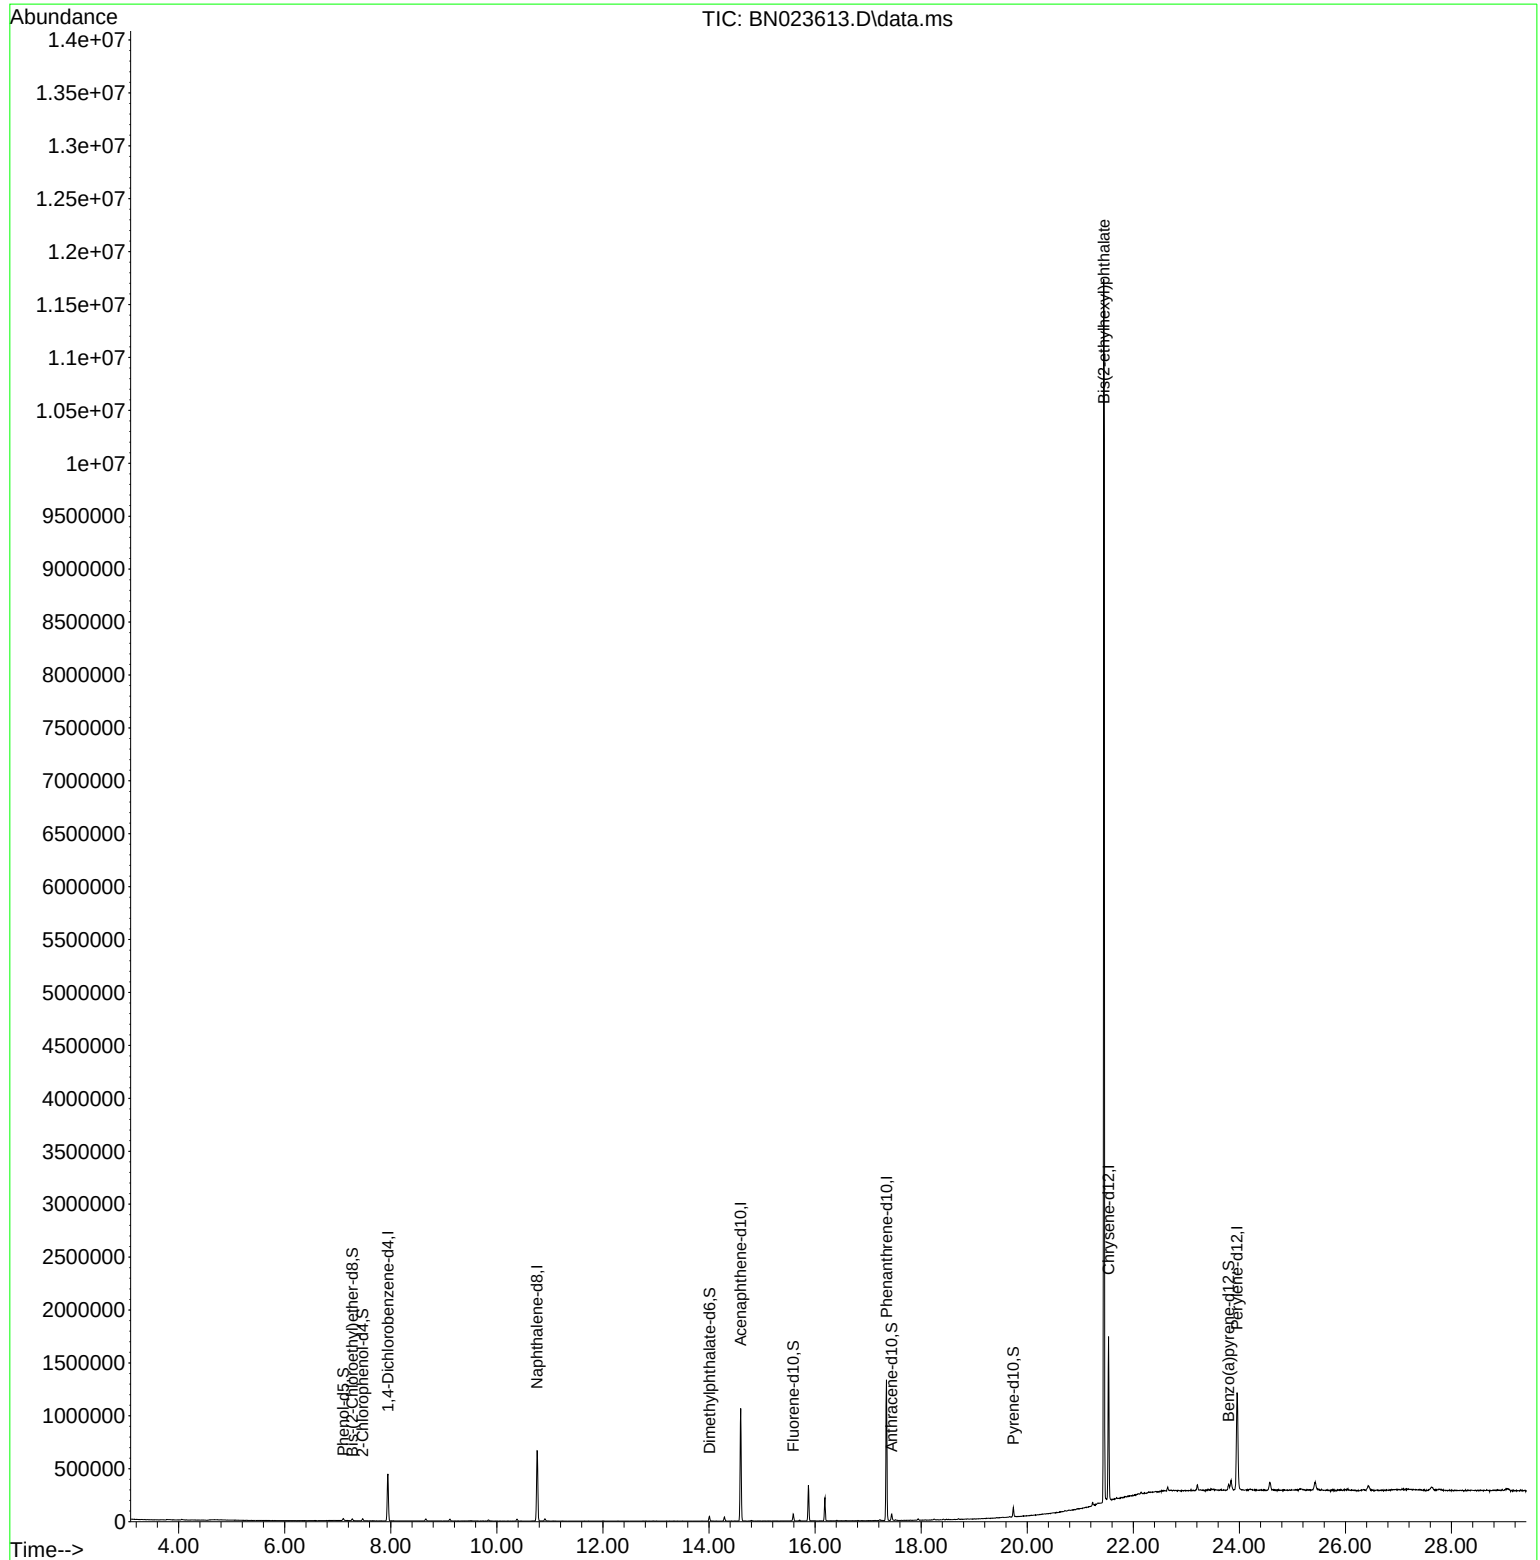

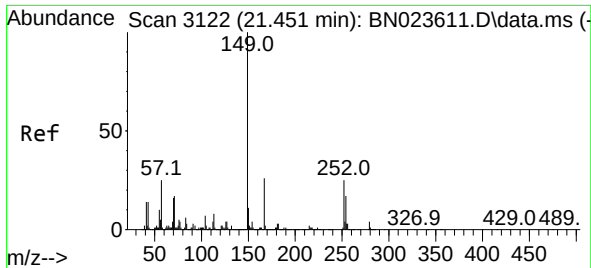

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 150.378 ng/ul
 RT: 21.445 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN023613.D
 Acq: 11 Jan 2023 15:53

Instrument :
 BNA_N
 ClientSampleId :
 A4477DL

Tgt Ion:149 Resp: 3883985
 Ion Ratio Lower Upper
 149 100
 167 27.5 22.0 33.0
 279 4.3 3.4 5.2

