

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
 Data File : BN023605.D
 Acq On : 11 Jan 2023 10:21
 Operator : CG/JU
 Sample : PB150058BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK058

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023605.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rVB	31187	43017	1.10%	0.108%
2	3.723	106	108	134	rBV	416866	744248	18.95%	1.870%
3	4.064	162	166	170	rBV	7327	9161	0.23%	0.023%
4	7.105	676	683	694	rVB	639730	974135	24.80%	2.448%
5	7.269	705	711	722	rVB	505978	788438	20.07%	1.981%
6	7.469	738	745	757	rVB	665164	998117	25.41%	2.508%
7	7.946	819	826	835	rBV	490040	776761	19.78%	1.952%
8	8.658	940	947	959	rBV	792160	1203440	30.64%	3.024%
9	9.116	1017	1025	1034	rBV	607059	970391	24.71%	2.438%
10	9.840	1140	1148	1159	rVB	514204	799555	20.36%	2.009%
11	10.375	1232	1239	1255	rBV	791198	1271265	32.37%	3.194%
12	10.758	1296	1304	1313	rBV	727401	1241143	31.60%	3.119%
13	10.899	1321	1328	1342	rBV	814767	1347940	34.32%	3.387%
14	12.346	1569	1574	1581	rBV	12551	19157	0.49%	0.048%
15	14.010	1850	1857	1868	rBV	1431818	1895886	48.27%	4.764%
16	14.293	1898	1905	1917	rBV	1607146	2248637	57.25%	5.650%
17	14.599	1950	1957	1965	rBV	1202451	1705154	43.41%	4.285%
18	14.793	1983	1990	2006	rBV	721374	960326	24.45%	2.413%
19	15.587	2117	2125	2132	rBV	2073635	2920096	74.35%	7.337%
20	15.640	2132	2134	2139	rVV5	3306	5256	0.13%	0.013%
21	15.704	2139	2145	2158	rVV	649203	875256	22.28%	2.199%
22	15.828	2161	2166	2173	rVB4	9745	14971	0.38%	0.038%
23	16.816	2328	2334	2336	rBV5	2312	3962	0.10%	0.010%
24	17.345	2418	2424	2430	rBV	1564063	2117421	53.91%	5.320%
25	17.445	2434	2441	2456	rBV	2423991	3265692	83.15%	8.206%
26	19.304	2753	2757	2762	rBV2	27083	34205	0.87%	0.086%
27	19.375	2765	2769	2773	rBV2	24507	32596	0.83%	0.082%
28	19.663	2816	2818	2822	rBV5	8584	10842	0.28%	0.027%
29	19.739	2825	2831	2840	rBV	2972460	3927685	100.00%	9.869%
30	21.533	3131	3136	3142	rBV	1895401	2367503	60.28%	5.949%
31	23.804	3515	3522	3538	rVB2	1976158	3900187	99.30%	9.800%
32	23.963	3542	3549	3560	rVB2	1190809	2325566	59.21%	5.843%




Sum of corrected areas: 39798009

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023605.D
Acq On : 11 Jan 2023 10:21
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

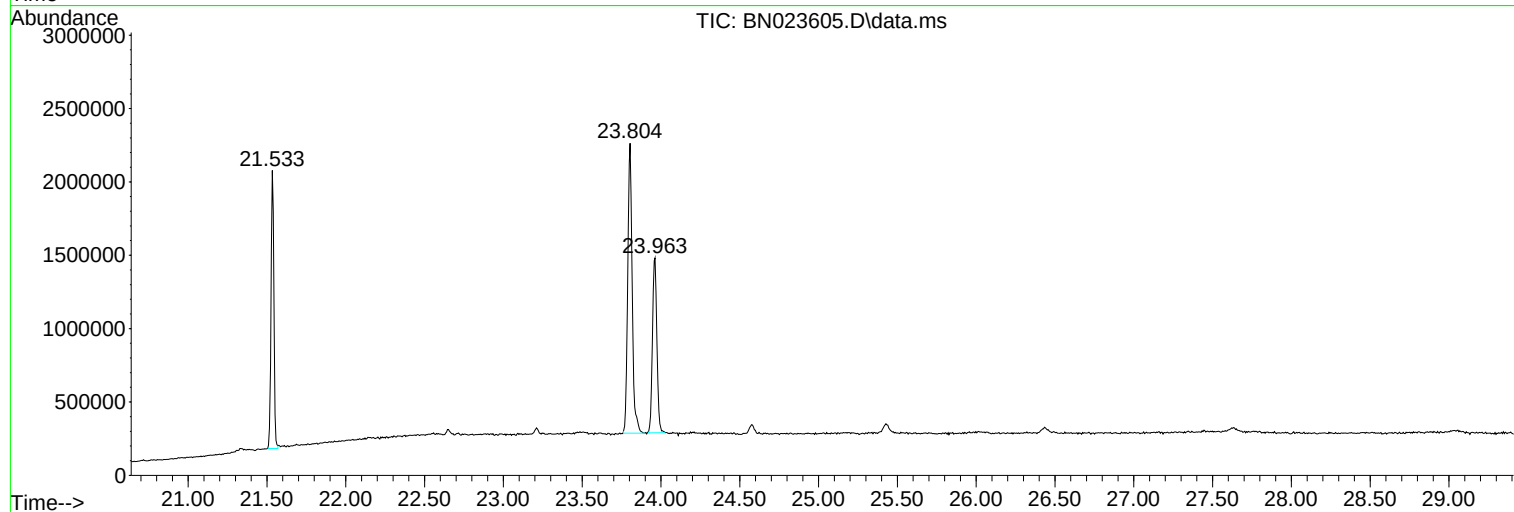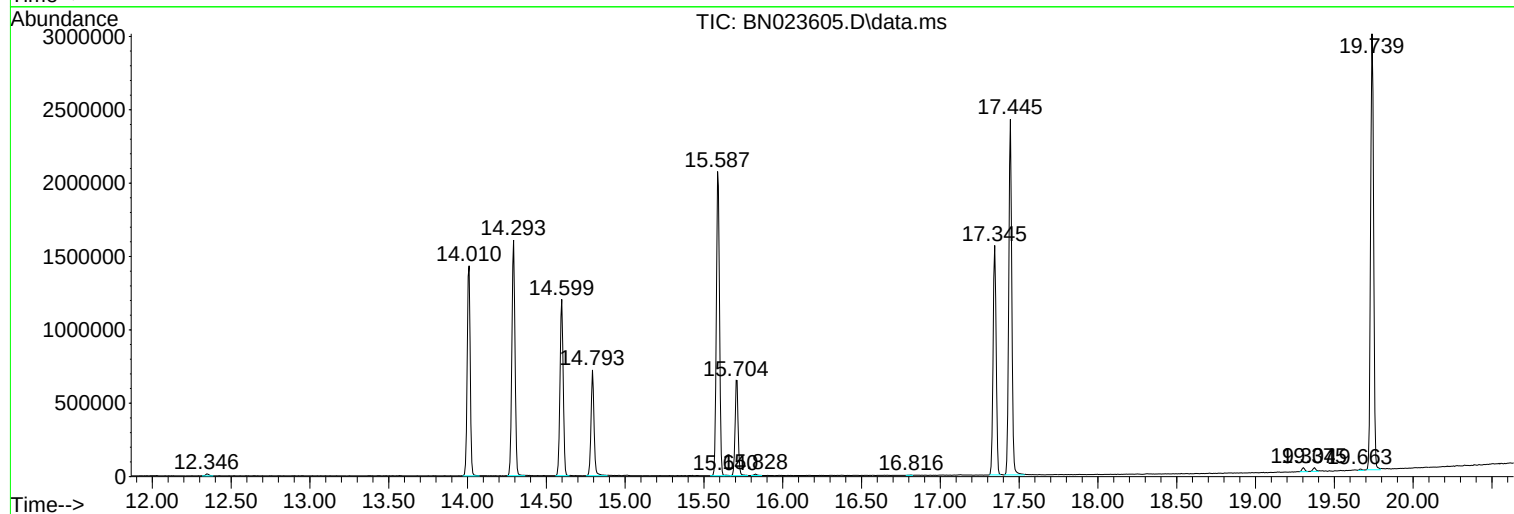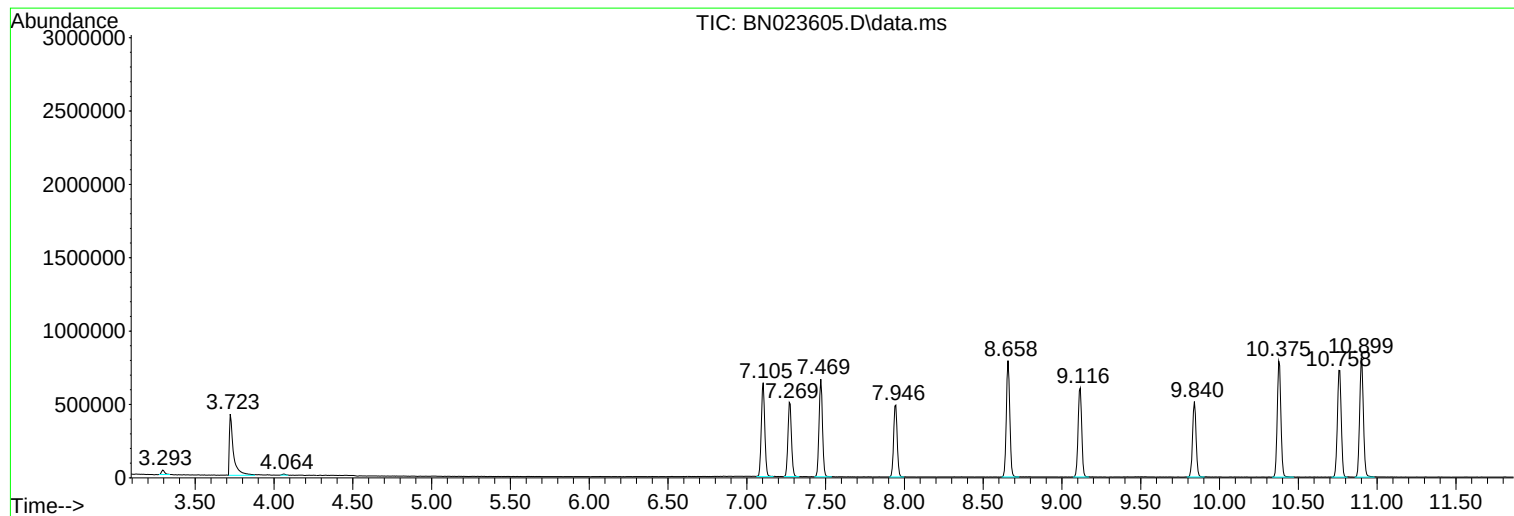

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023605.D
Acq On : 11 Jan 2023 10:21
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023605.D
Acq On : 11 Jan 2023 10:21
Operator : CG/JU
Sample : PB150058BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK058

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc