

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
 Data File : BN023607.D
 Acq On : 11 Jan 2023 11:36
 Operator : CG/JU
 Sample : PB150061BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK061

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023607.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.299	32	36	42	rBV	31784	45646	0.96%	0.101%
2	3.722	105	108	135	rBV	460401	821412	17.36%	1.826%
3	4.064	162	166	177	rVB2	10848	21448	0.45%	0.048%
4	7.105	677	683	692	rVB	702230	1062296	22.46%	2.361%
5	7.275	705	712	721	rVB	546175	865218	18.29%	1.923%
6	7.469	739	745	754	rBV	725449	1103283	23.32%	2.452%
7	7.946	819	826	835	rVB	553146	874858	18.49%	1.945%
8	8.657	940	947	959	rBV	873730	1330410	28.12%	2.957%
9	9.116	1017	1025	1037	rVB	685353	1069398	22.61%	2.377%
10	9.840	1139	1148	1158	rBV	572010	888377	18.78%	1.975%
11	10.381	1232	1240	1250	rBV	873033	1389754	29.38%	3.089%
12	10.757	1297	1304	1312	rBV	829320	1395134	29.49%	3.101%
13	10.898	1322	1328	1343	rBV	898087	1486894	31.43%	3.305%
14	12.351	1570	1575	1581	rVB	12853	20143	0.43%	0.045%
15	14.010	1850	1857	1867	rVB	1546582	2080624	43.98%	4.625%
16	14.292	1898	1905	1920	rBV	1776982	2457794	51.96%	5.463%
17	14.598	1950	1957	1967	rVB	1360833	1914888	40.48%	4.257%
18	14.792	1984	1990	2004	rBV	827377	1106669	23.39%	2.460%
19	15.592	2119	2126	2133	rBV	2285121	3222241	68.12%	7.163%
20	15.710	2140	2146	2155	rBV	753379	998580	21.11%	2.220%
21	15.828	2162	2166	2172	rVB4	10049	14978	0.32%	0.033%
22	16.810	2328	2333	2337	rBV4	2638	5226	0.11%	0.012%
23	17.133	2381	2388	2393	rBV4	3514	8154	0.17%	0.018%
24	17.345	2417	2424	2431	rBV	1756209	2379235	50.29%	5.289%
25	17.445	2435	2441	2458	rVV	2755904	3629968	76.73%	8.069%
26	19.304	2753	2757	2762	rBV2	29507	40316	0.85%	0.090%
27	19.375	2765	2769	2774	rVV	29424	37938	0.80%	0.084%
28	19.739	2825	2831	2839	rBV	3438338	4402229	93.06%	9.786%
29	21.533	3131	3136	3143	rBV	2262402	2763006	58.41%	6.142%
30	23.804	3515	3522	3535	rVB	2308334	4730563	100.00%	10.516%
31	23.962	3542	3549	3560	rVB2	1423072	2819439	59.60%	6.267%




Sum of corrected areas: 44986119

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023607.D
Acq On : 11 Jan 2023 11:36
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

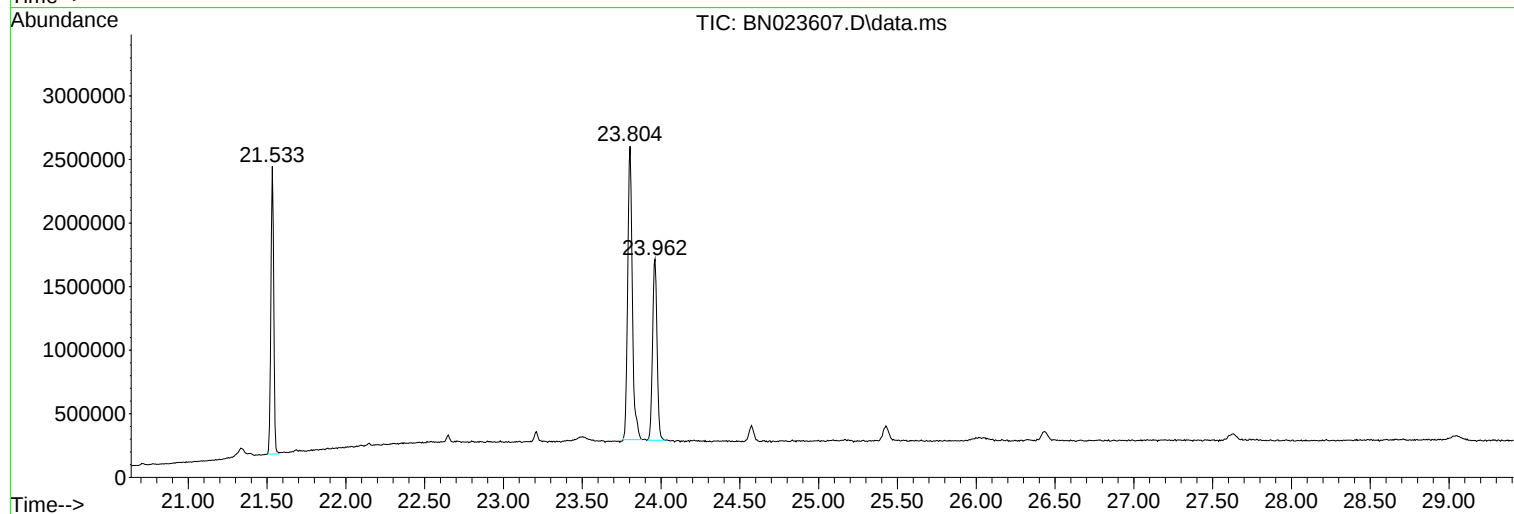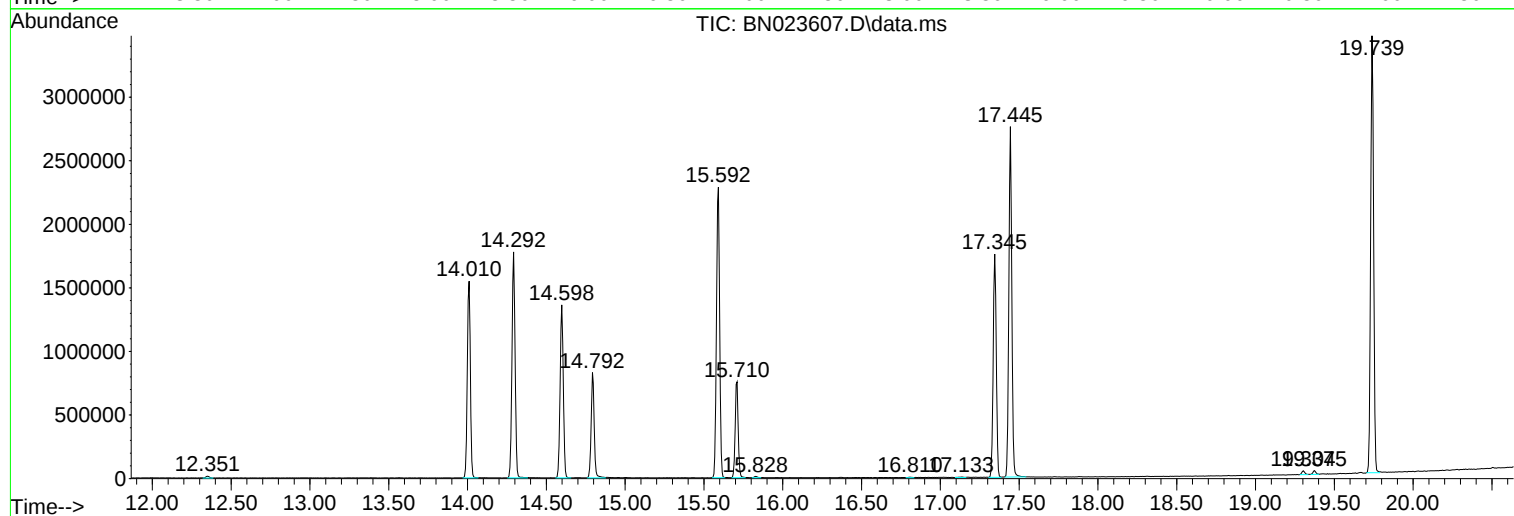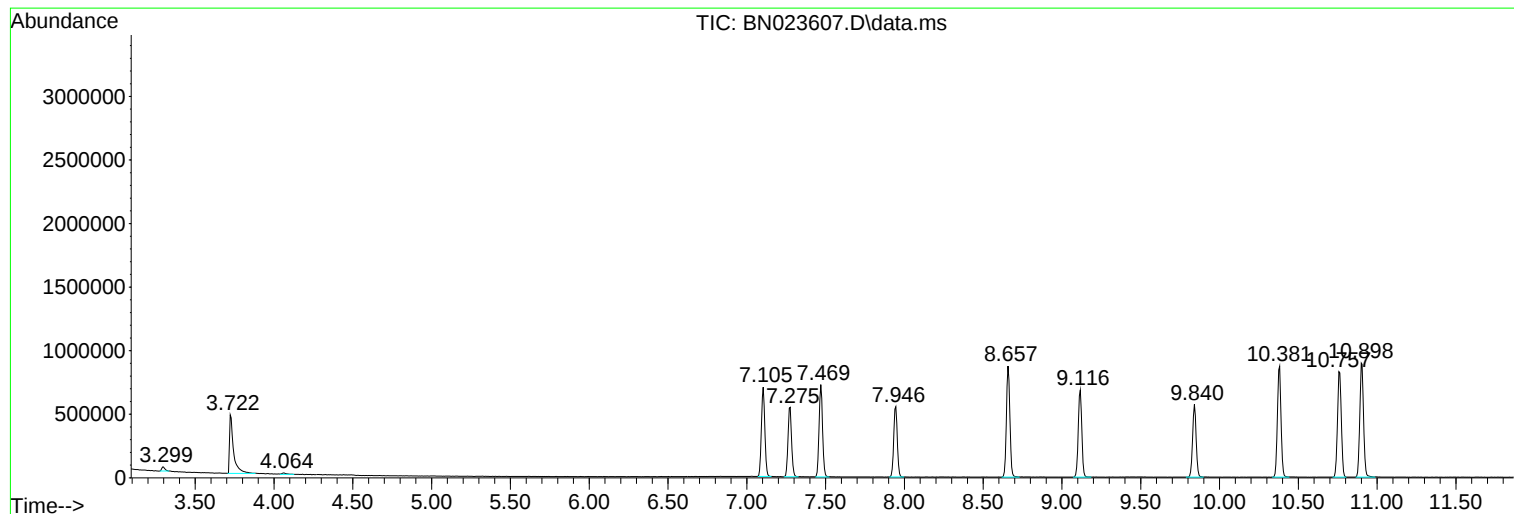

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023607.D
Acq On : 11 Jan 2023 11:36
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023607.D
Acq On : 11 Jan 2023 11:36
Operator : CG/JU
Sample : PB150061BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK061

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------