

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
 Data File : BN023612.D
 Acq On : 11 Jan 2023 15:16
 Operator : CG/JU
 Sample : PB150112BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK112

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023612.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	44	rVB	36445	53244	1.22%	0.111%
2	3.722	105	108	135	rBV	481153	822964	18.79%	1.719%
3	4.058	162	165	170	rBV	9314	13236	0.30%	0.028%
4	7.105	676	683	693	rVB	716790	1091255	24.92%	2.280%
5	7.269	705	711	721	rBV	576582	894730	20.43%	1.869%
6	7.469	738	745	756	rBV	730443	1127624	25.75%	2.355%
7	7.946	819	826	835	rVB	690832	1092668	24.95%	2.282%
8	8.657	940	947	958	rBV	912121	1388430	31.70%	2.900%
9	9.110	1016	1024	1039	rBV	684899	1110269	25.35%	2.319%
10	9.840	1141	1148	1157	rBV	596998	931758	21.28%	1.946%
11	10.375	1232	1239	1250	rBV	900313	1447346	33.05%	3.023%
12	10.757	1297	1304	1313	rVB	1059613	1752534	40.02%	3.661%
13	10.899	1321	1328	1344	rBV	936248	1549489	35.38%	3.237%
14	12.351	1570	1575	1585	rVB2	15439	23592	0.54%	0.049%
15	14.010	1850	1857	1866	rVB	1657681	2231333	50.95%	4.661%
16	14.292	1898	1905	1916	rBV	1856578	2617988	59.78%	5.469%
17	14.598	1950	1957	1968	rBV	1708967	2411090	55.06%	5.037%
18	14.792	1984	1990	2002	rBV	860587	1147666	26.21%	2.397%
19	15.016	2023	2028	2031	rVB6	3488	5687	0.13%	0.012%
20	15.587	2119	2125	2138	rBV	2327912	3349893	76.49%	6.998%
21	15.710	2139	2146	2158	rVV	797710	1062143	24.25%	2.219%
22	15.828	2161	2166	2170	rVB2	10533	14542	0.33%	0.030%
23	17.345	2417	2424	2431	rBV	2145589	2943171	67.20%	6.148%
24	17.445	2434	2441	2465	rVV	2790162	3766698	86.01%	7.868%
25	19.304	2753	2757	2763	rBV2	32416	45596	1.04%	0.095%
26	19.375	2765	2769	2773	rVV	29231	36945	0.84%	0.077%
27	19.739	2825	2831	2837	rBV	3423085	4379402	100.00%	9.148%
28	21.533	3131	3136	3144	rBV	2456350	3146008	71.84%	6.572%
29	23.804	3515	3522	3536	rVB	2155133	4321629	98.68%	9.027%
30	23.963	3542	3549	3567	rVB2	1543957	3093146	70.63%	6.461%




Sum of corrected areas: 47872076

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023612.D
Acq On : 11 Jan 2023 15:16
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

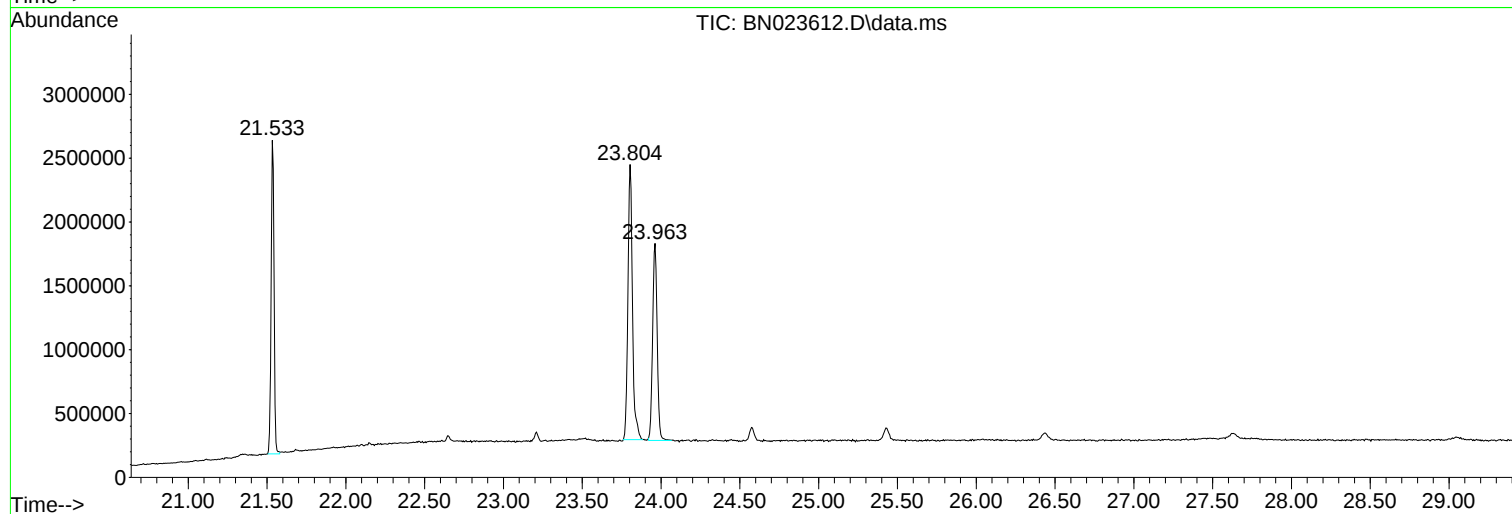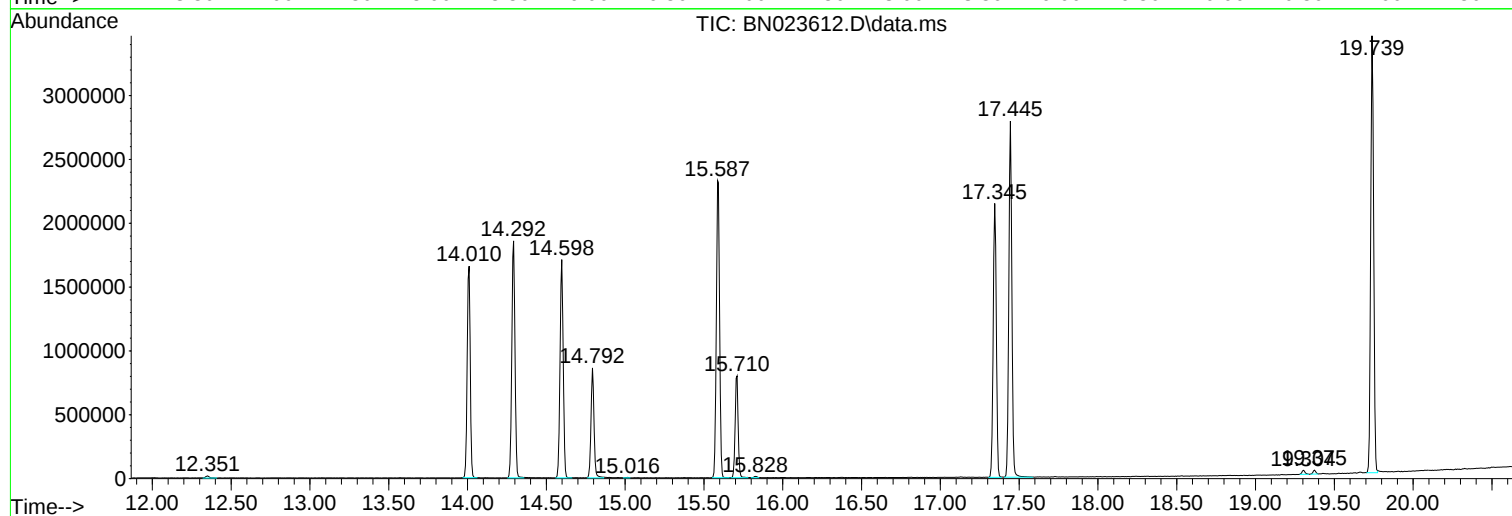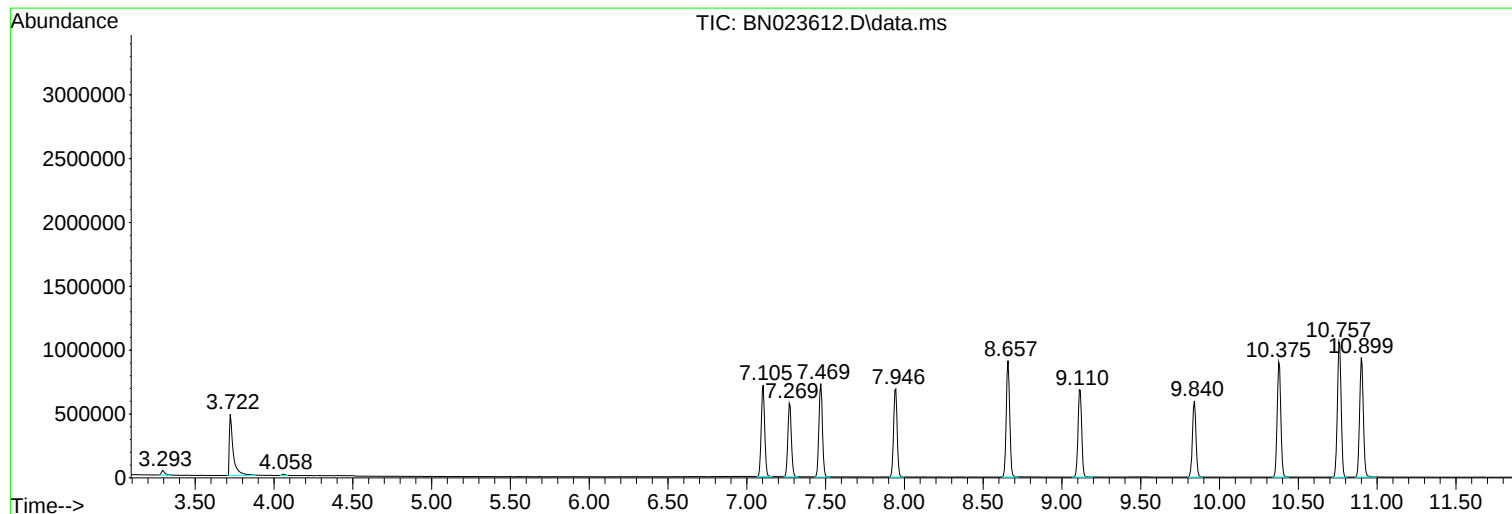

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023612.D
Acq On : 11 Jan 2023 15:16
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011123\
Data File : BN023612.D
Acq On : 11 Jan 2023 15:16
Operator : CG/JU
Sample : PB150112BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK112

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc