

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
 Data File : BN018387.D
 Acq On : 12 Jan 2022 10:18
 Operator : CG/JU
 Sample : PB141951BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK951

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018387.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.058	8	12	18	rBV	117734	158172	1.58%	0.130%
2	3.458	78	80	97	rBV	1591488	2465234	24.63%	2.022%
3	3.799	134	138	143	rBV2	34138	44823	0.45%	0.037%
4	6.775	637	644	659	rBV	1964633	3123713	31.22%	2.562%
5	6.928	664	670	681	rVV	1659996	2577916	25.76%	2.114%
6	7.122	697	703	715	rBV	2010170	3191645	31.89%	2.617%
7	7.587	776	782	792	rBV	1955281	3035824	30.34%	2.489%
8	8.305	898	904	921	rBV	2370601	3819434	38.17%	3.132%
9	8.734	971	977	995	rBV	1826893	3010087	30.08%	2.468%
10	9.457	1093	1100	1116	rBV	1595531	2551166	25.49%	2.092%
11	9.999	1185	1192	1206	rBV	2160230	3703334	37.01%	3.037%
12	10.369	1247	1255	1267	rBV	2724156	4521859	45.19%	3.708%
13	10.505	1271	1278	1302	rBV	2209968	4062824	40.60%	3.332%
14	11.981	1524	1529	1537	rBV4	26134	49372	0.49%	0.040%
15	13.651	1807	1813	1828	rBV	4284927	5865508	58.61%	4.810%
16	13.922	1852	1859	1875	rBV	4793287	6988617	69.84%	5.731%
17	14.234	1905	1912	1920	rBV	4138342	5910590	59.06%	4.847%
18	14.445	1942	1948	1969	rBV	1147022	2263499	22.62%	1.856%
19	15.228	2074	2081	2096	rBV	5958166	8433549	84.28%	6.916%
20	15.357	2096	2103	2116	rVV	1656977	2430888	24.29%	1.993%
21	15.469	2118	2122	2127	rVB2	29557	45888	0.46%	0.038%
22	16.763	2339	2342	2352	rVB2	20292	29899	0.30%	0.025%
23	16.975	2372	2378	2389	rBV	4917223	6899364	68.95%	5.658%
24	17.075	2389	2395	2417	rVB	6419456	9102405	90.96%	7.464%
25	18.939	2708	2712	2719	rBV2	69513	96837	0.97%	0.079%
26	19.016	2719	2725	2729	rBV	58721	90406	0.90%	0.074%
27	19.375	2780	2786	2804	rBV	7313216	10007040	100.00%	8.206%
28	21.175	3086	3092	3102	rBV	5362722	7223898	72.19%	5.924%
29	21.780	3192	3195	3200	rBV4	57417	75221	0.75%	0.062%
30	22.245	3270	3274	3280	rBV2	114793	150414	1.50%	0.123%
31	22.751	3355	3360	3371	rVB2	166859	283266	2.83%	0.232%
32	23.251	3437	3445	3452	rBV2	5205054	9837276	98.30%	8.067%
33	23.316	3453	3456	3461	rVV	309078	542180	5.42%	0.445%
34	23.392	3462	3469	3486	rVB2	4001131	7611182	76.06%	6.241%
35	23.969	3561	3567	3576	rBV2	237198	499685	4.99%	0.410%
36	24.721	3688	3695	3704	rBV2	222740	545870	5.45%	0.448%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018387.D
Acq On : 12 Jan 2022 10:18
Operator : CG/JU
Sample : PB141951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK951

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Title : SVOA CALIBRATION

37	25.610	3838	3846	3856	rVB2	167045	444441	4.44%	0.364%
38	26.645	4017	4022	4030	rVB3	101168	255179	2.55%	0.209%


Sum of corrected areas: 121948505

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018387.D
Acq On : 12 Jan 2022 10:18
Operator : CG/JU
Sample : PB141951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK951

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

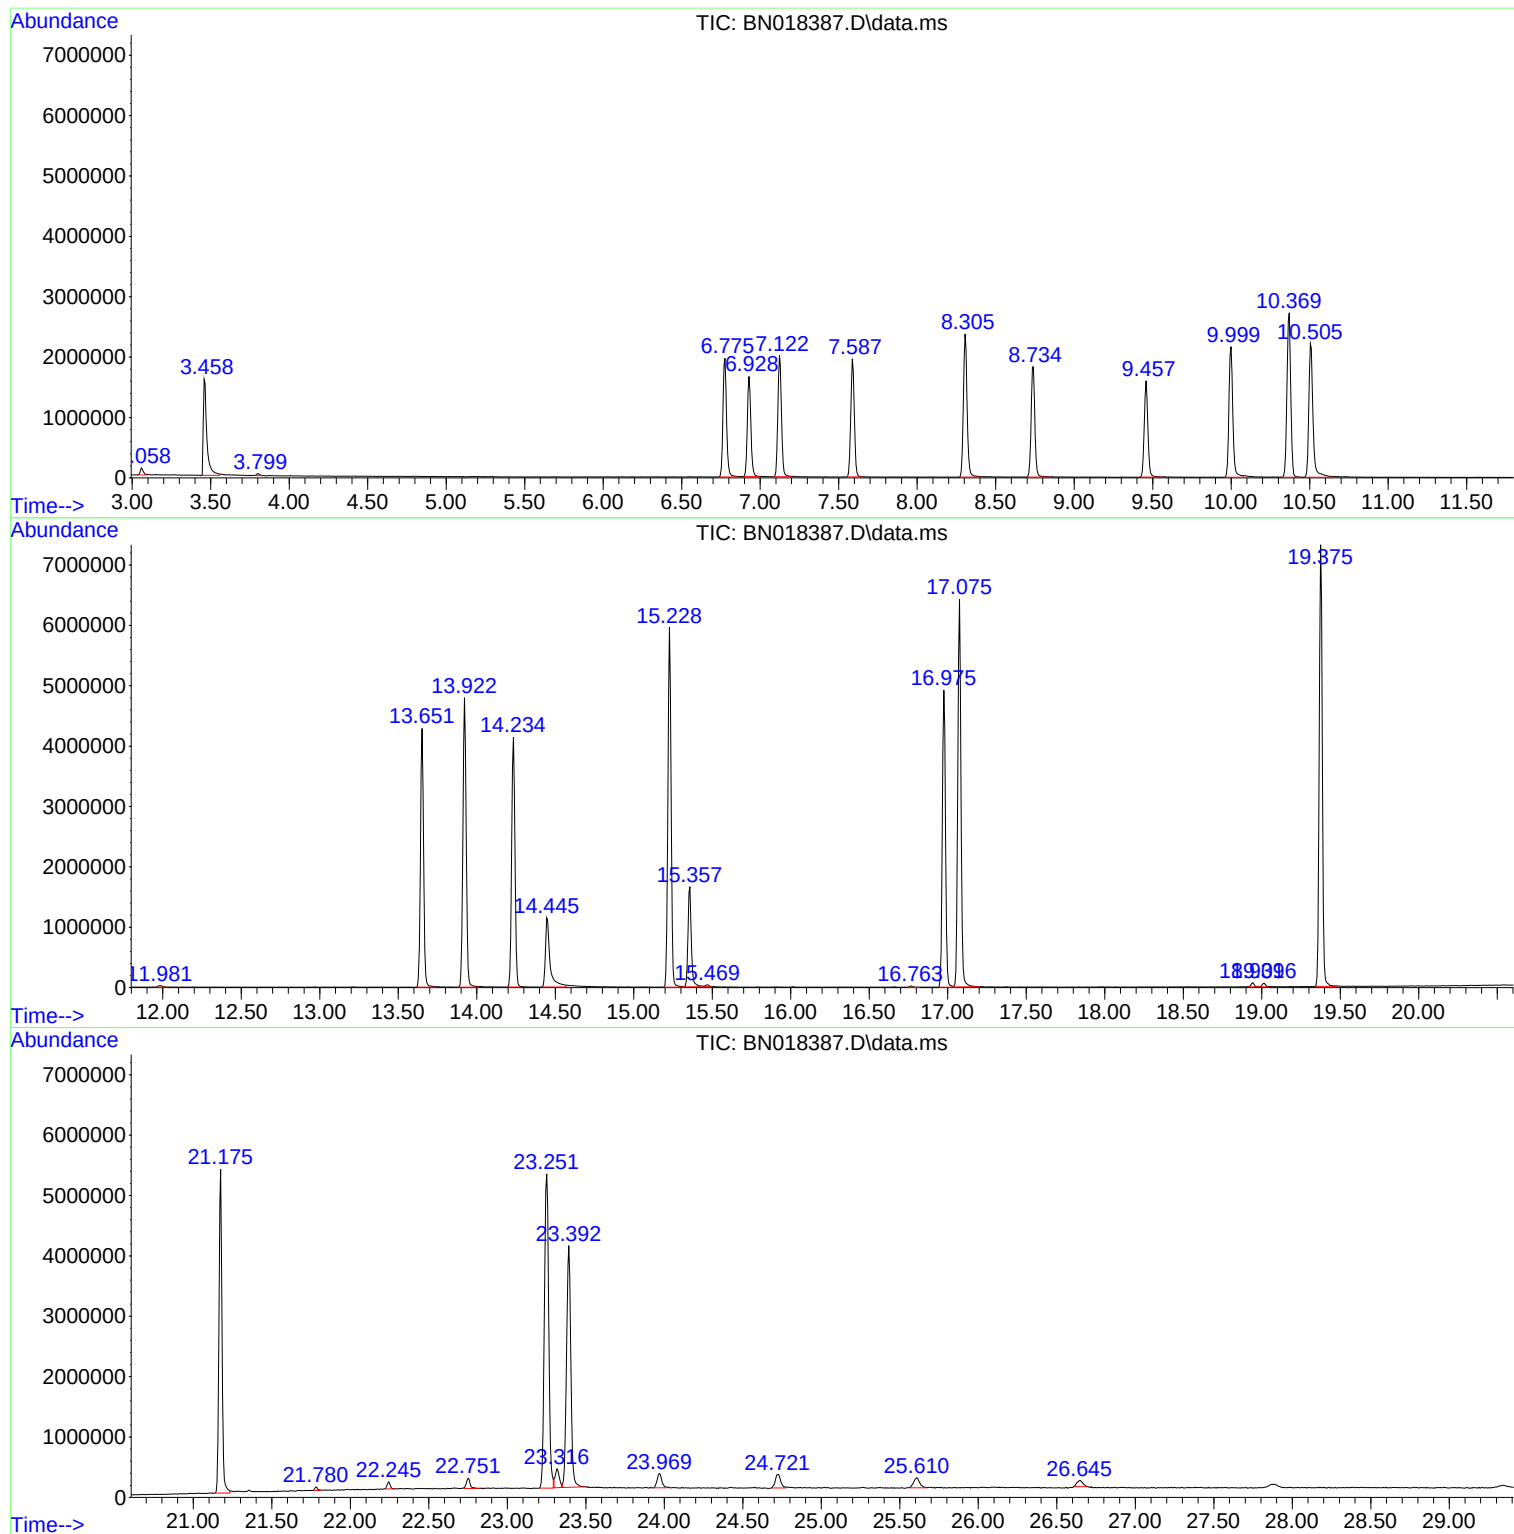

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018387.D
Acq On : 12 Jan 2022 10:18
Operator : CG/JU
Sample : PB141951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK951

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018387.D
Acq On : 12 Jan 2022 10:18
Operator : CG/JU
Sample : PB141951BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK951

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------