

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
 Data File : BN018389.D
 Acq On : 12 Jan 2022 12:22
 Operator : CG/JU
 Sample : PB141976BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

Signal : TIC: BN018389.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.052	7	11	18	rBV	129814	180875	1.45%	0.128%
2	3.452	77	79	98	rBV	1984170	3026907	24.34%	2.138%
3	3.793	133	137	145	rVB3	40095	62288	0.50%	0.044%
4	4.787	302	306	312	rBV6	9553	18164	0.15%	0.013%
5	6.764	635	642	658	rBV	2498392	3859369	31.04%	2.726%
6	6.922	662	669	685	rVB	1960052	3186064	25.62%	2.251%
7	7.116	695	702	716	rBV	2473002	3900012	31.36%	2.755%
8	7.581	774	781	792	rBV	2048894	3208263	25.80%	2.266%
9	8.299	896	903	918	rBV	2959694	4694339	37.75%	3.316%
10	8.728	969	976	994	rBV	2332676	3687637	29.66%	2.605%
11	9.452	1091	1099	1116	rBV	1945769	3180836	25.58%	2.247%
12	9.993	1184	1191	1202	rBV	2727187	4577384	36.81%	3.233%
13	10.363	1246	1254	1265	rBV	2810619	4693073	37.74%	3.315%
14	10.499	1269	1277	1296	rBV	2758510	4836967	38.90%	3.417%
15	11.963	1521	1526	1534	rBV2	34286	73968	0.59%	0.052%
16	13.204	1733	1737	1741	rBV3	8354	13979	0.11%	0.010%
17	13.651	1806	1813	1828	rBV	4919317	7015122	56.42%	4.955%
18	13.922	1852	1859	1882	rBV	5657396	8407598	67.61%	5.939%
19	14.228	1905	1911	1924	rBV	4089796	6152797	49.48%	4.346%
20	14.445	1942	1948	1968	rBV	1824417	3115460	25.05%	2.201%
21	15.228	2074	2081	2094	rBV	6953722	9904982	79.66%	6.997%
22	15.351	2096	2102	2118	rVV	2305239	3274312	26.33%	2.313%
23	15.469	2118	2122	2128	rVB3	38178	66024	0.53%	0.047%
24	15.798	2173	2178	2183	rVB9	8069	15417	0.12%	0.011%
25	16.769	2336	2343	2346	rBV3	20344	32039	0.26%	0.023%
26	16.975	2371	2378	2388	rBV	5056826	7089999	57.02%	5.008%
27	17.075	2388	2395	2413	rVV	7456063	10750319	86.45%	7.594%
28	17.963	2540	2546	2553	rVB6	10144	23136	0.19%	0.016%
29	18.204	2583	2587	2592	rBV6	14555	21135	0.17%	0.015%
30	18.939	2708	2712	2717	rBV2	90415	122643	0.99%	0.087%
31	19.016	2720	2725	2730	rVB	86771	125859	1.01%	0.089%
32	19.375	2780	2786	2798	rBV	8805209	12131107	97.56%	8.569%
33	20.410	2958	2962	2966	rBV3	21978	25155	0.20%	0.018%
34	20.457	2966	2970	2973	rBV3	23456	28600	0.23%	0.020%
35	20.692	3008	3010	3015	rVB4	28617	33302	0.27%	0.024%
36	20.763	3020	3022	3026	rVB4	37250	45206	0.36%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
 Data File : BN018389.D
 Acq On : 12 Jan 2022 12:22
 Operator : CG/JU
 Sample : PB141976BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK976

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
 Title : SVOA CALIBRATION

37	21.016	3061	3065	3068	rBV6	26608	33893	0.27%	0.024%
38	21.175	3087	3092	3110	rBV	5815916	7376479	59.32%	5.211%
39	21.357	3121	3123	3127	rVB3	31133	33748	0.27%	0.024%
40	21.786	3193	3196	3200	rBV2	52115	62358	0.50%	0.044%
41	22.251	3270	3275	3282	rBV2	110605	182656	1.47%	0.129%
42	22.757	3357	3361	3367	rVB	138749	194328	1.56%	0.137%
43	23.257	3438	3446	3454	rBV	6718791	12434810	100.00%	8.784%
44	23.321	3454	3457	3462	rVV	241512	460063	3.70%	0.325%
45	23.398	3462	3470	3489	rVB2	4110515	7959680	64.01%	5.623%
46	23.974	3563	3568	3580	rVB2	197323	417917	3.36%	0.295%
47	24.727	3691	3696	3707	rVB	170488	370298	2.98%	0.262%
48	25.615	3841	3847	3854	rBV2	105199	249975	2.01%	0.177%
49	26.657	4019	4024	4033	rVB5	75280	208942	1.68%	0.148%




Sum of corrected areas: 141565484

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018389.D
Acq On : 12 Jan 2022 12:22
Operator : CG/JU
Sample : PB141976BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

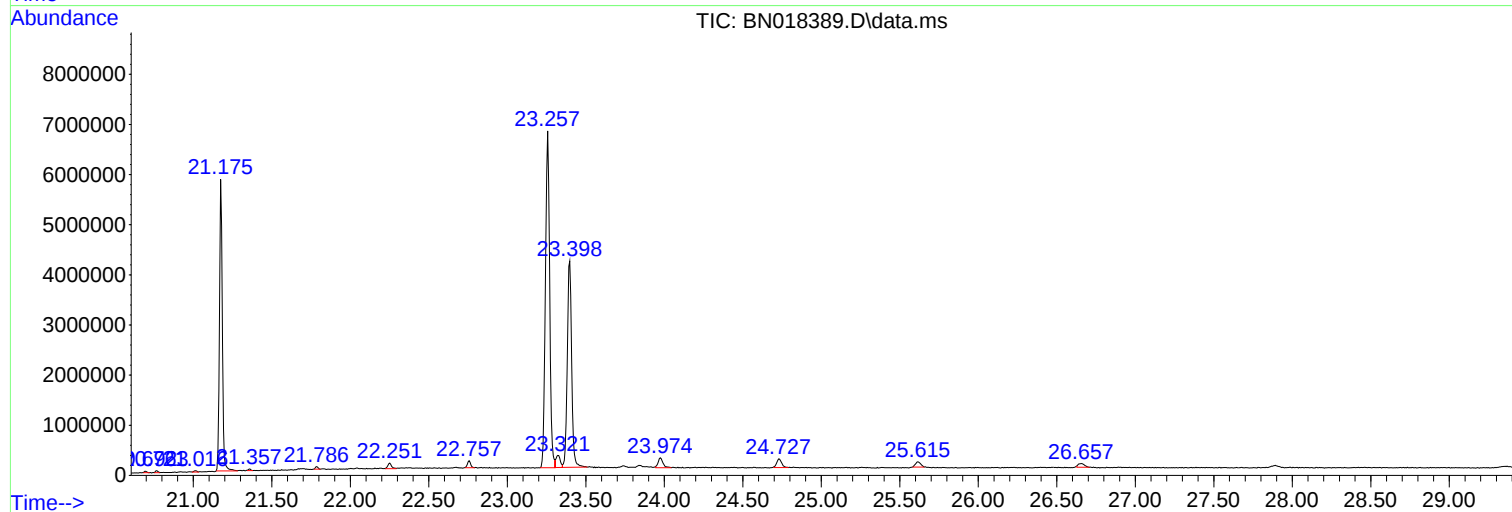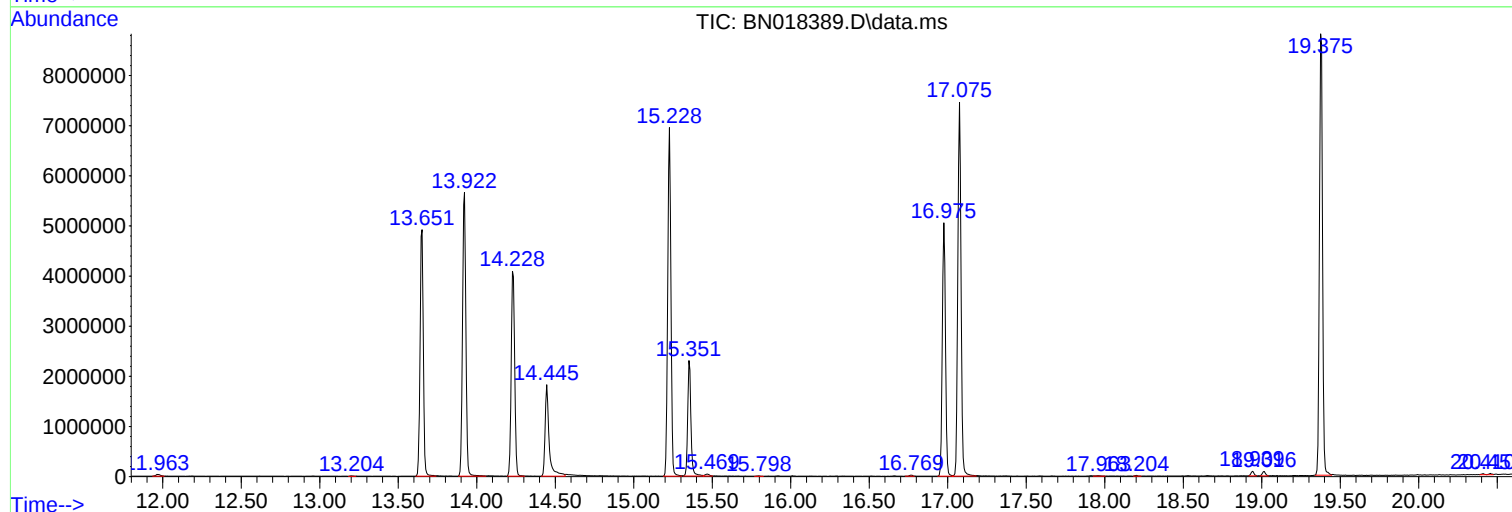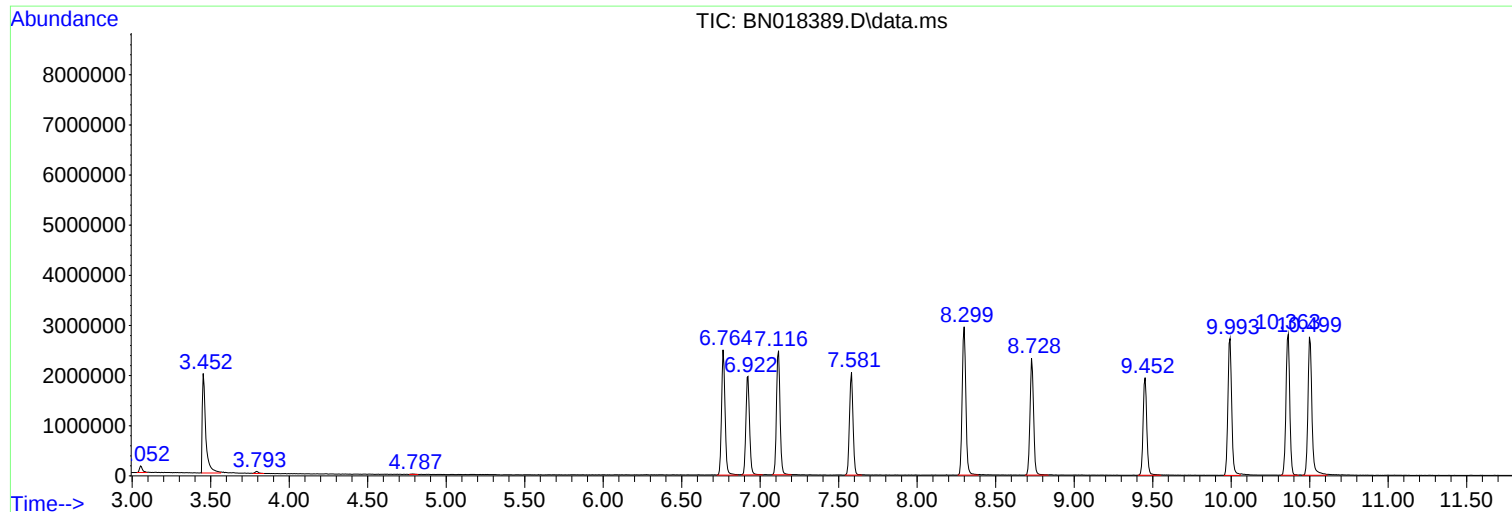

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018389.D
Acq On : 12 Jan 2022 12:22
Operator : CG/JU
Sample : PB141976BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011222\
Data File : BN018389.D
Acq On : 12 Jan 2022 12:22
Operator : CG/JU
Sample : PB141976BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK976

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------