

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
 Data File : BN023647.D
 Acq On : 12 Jan 2023 16:47
 Operator : CG/JU
 Sample : 01050-04ME
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4477ME

Quant Time: Jan 12 17:34:47 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	182154	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.758	136	858162	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.598	164	535634	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	1161281	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1075789	20.000	ng/u1	-0.01
88) Perylene-d12	23.963	264	1166947	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	28335	6.694	ng/uL	0.00
4) Pyridine-d5	3.723	84	422272	33.249	ng/u1	0.00
7) Phenol-d5	7.099	99	603131	37.360	ng/u1	-0.01
9) Bis-(2-Chloroethyl)eth...	7.269	67	385900	38.965	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	490435	39.666	ng/u1	0.00
15) 4-Methylphenol-d8	8.658	113	493430	38.294	ng/u1	-0.01
21) Nitrobenzene-d5	9.111	128	249437	38.546	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.840	143	268080	39.134	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	474871	36.343	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.899	131	698085	33.965	ng/u1	-0.01
46) Dimethylphthalate-d6	14.010	166	1443762	36.234	ng/u1	0.00
49) Acenaphthylene-d8	14.293	160	1701882	38.549	ng/u1	0.00
54) 4-Nitrophenol-d4	14.793	143	264602	32.620	ng/u1	-0.01
60) Fluorene-d10	15.587	176	1280950	37.623	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.710	200	195824	27.953	ng/u1	0.00
73) Anthracene-d10	17.445	188	2017123	38.816	ng/u1	0.00
81) Pyrene-d10	19.739	212	2377695	38.646	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.810	264	2218456	38.442	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.451	149	9020507	206.457	ng/u1#	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023647.D
Acq On : 12 Jan 2023 16:47
Operator : CG/JU
Sample : 01050-04ME
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4477ME

Quant Time: Jan 12 17:34:47 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 05 03:34:47 2023
Response via : Initial Calibration

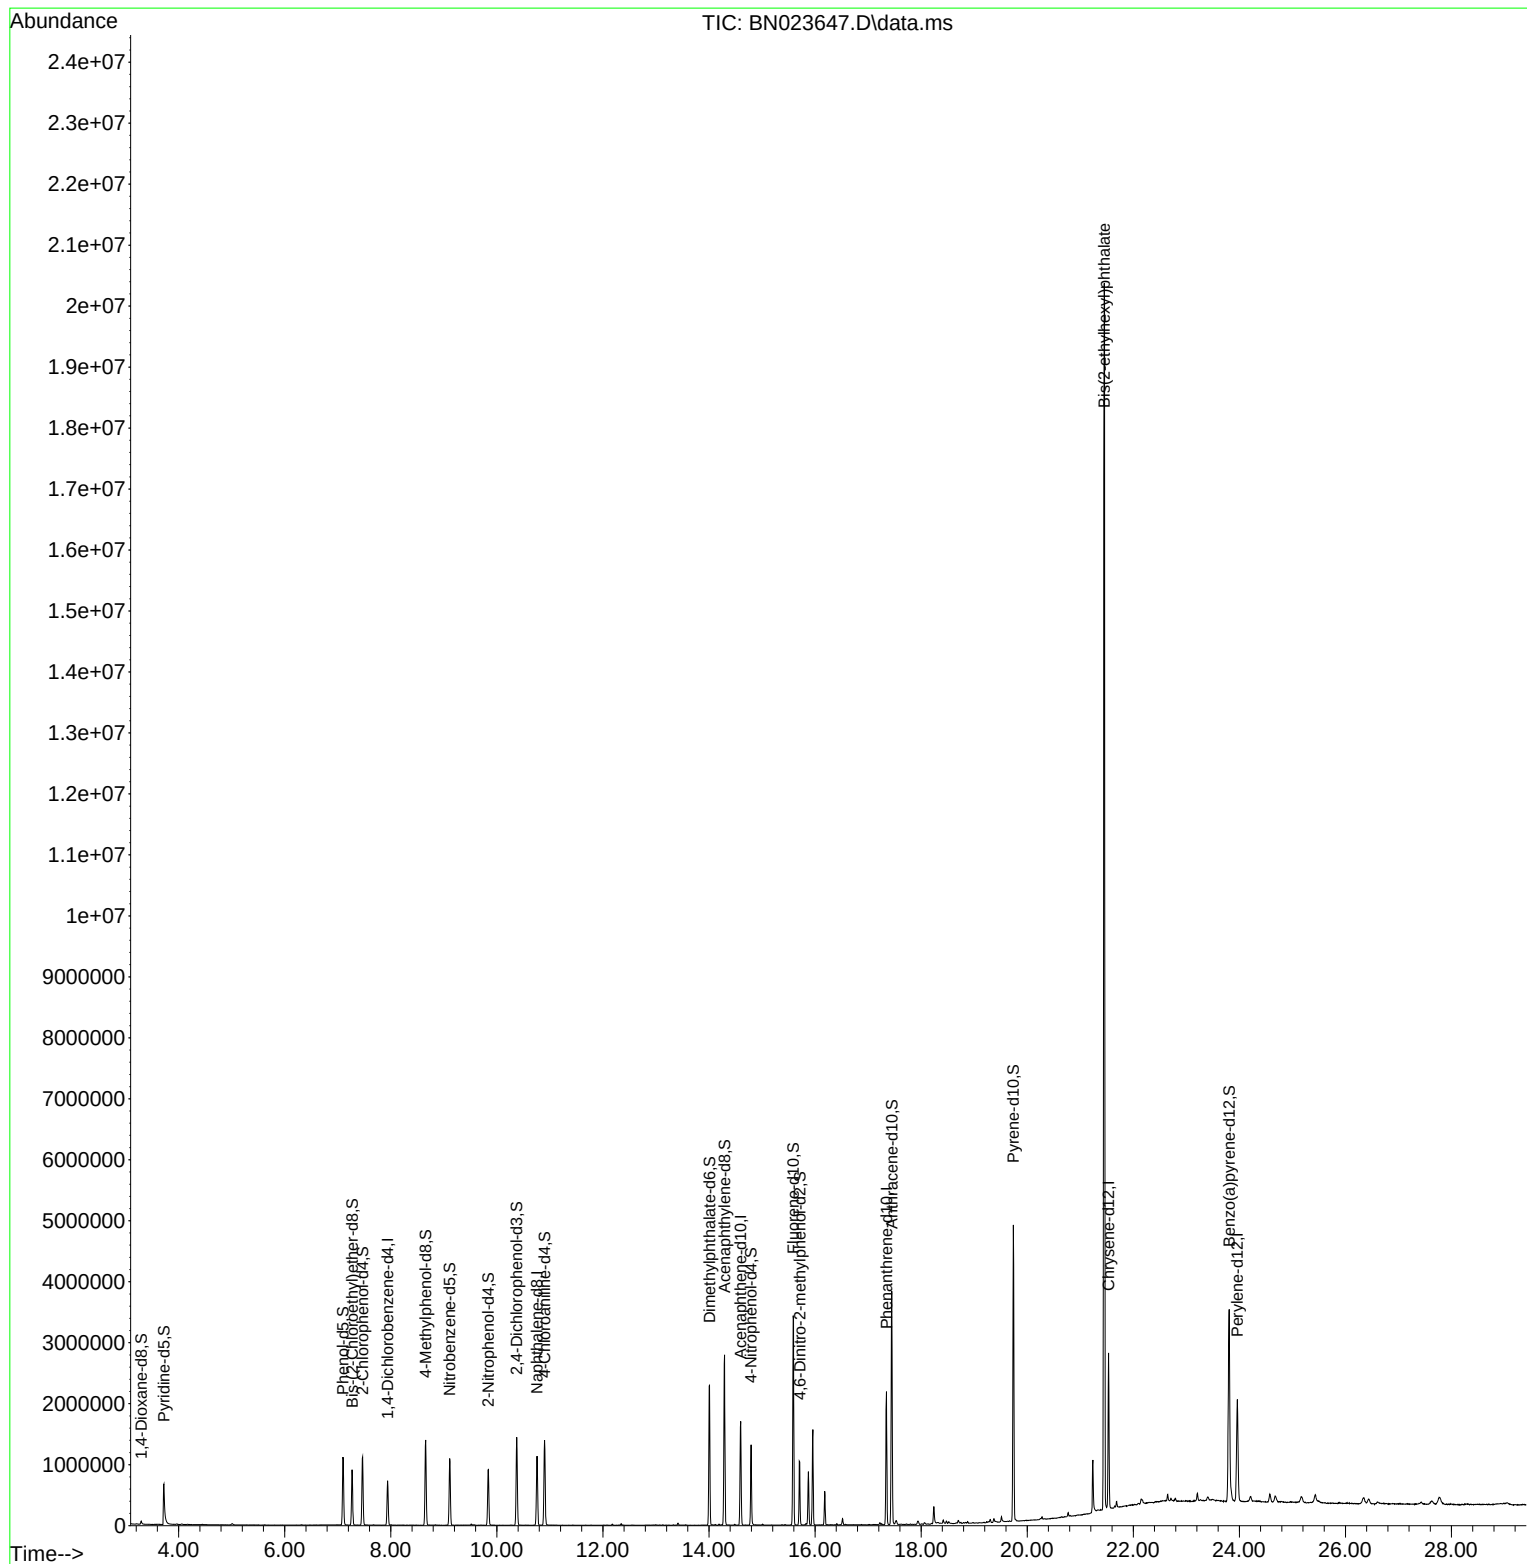

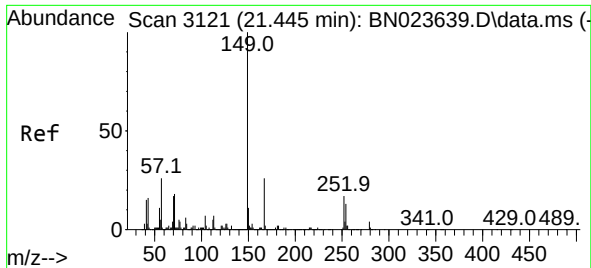

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 206.457 ng/ul
 RT: 21.451 min Scan# 31
 Delta R.T. 0.000 min
 Lab File: BN023647.D
 Acq: 12 Jan 2023 16:47

Instrument :
 BNA_N
 ClientSampleId :
 A4477ME

Tgt Ion:149 Resp: 9020507
 Ion Ratio Lower Upper
 149 100
 167 29.1 22.0 33.0
 279 5.3 3.4 5.2#

