

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
 Data File : BN023648.D
 Acq On : 12 Jan 2023 17:24
 Operator : CG/JU
 Sample : 01050-04MEDL 10X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4477MEDL

Quant Time: Jan 12 17:55:16 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Jan 05 03:34:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.940	152	186118	20.000	ng/u1	-0.01
20) Naphthalene-d8	10.757	136	859636	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.598	164	535601	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.345	188	1167920	20.000	ng/u1	0.00
79) Chrysene-d12	21.533	240	1063422	20.000	ng/u1	-0.01
88) Perylene-d12	23.963	264	1086401	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.293	96	3272	0.757	ng/uL	0.00
4) Pyridine-d5	3.740	84	33077	2.549	ng/u1	0.01
7) Phenol-d5	7.105	99	53357	3.235	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.269	67	37344	3.690	ng/u1	0.00
11) 2-Chlorophenol-d4	7.469	132	43250	3.424	ng/u1	0.00
15) 4-Methylphenol-d8	8.658	113	41835	3.178	ng/u1	-0.01
21) Nitrobenzene-d5	9.110	128	19909	3.071	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.840	143	18372	2.677	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.375	165	38903	2.972	ng/u1	-0.01
31) 4-Chloroaniline-d4	10.904	131	61806	3.002	ng/u1	0.00
46) Dimethylphthalate-d6	14.004	166	131998	3.313	ng/u1	-0.01
49) Acenaphthylene-d8	14.287	160	132460	3.001	ng/u1	-0.01
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/u1	
60) Fluorene-d10	15.587	176	119582	3.512	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/u1	
73) Anthracene-d10	17.445	188	181254	3.468	ng/u1	0.00
81) Pyrene-d10	19.739	212	218105	3.586	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.798	264	189001	3.518	ng/u1	-0.01
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.445	149	1170630	27.104	ng/u1	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023648.D
Acq On : 12 Jan 2023 17:24
Operator : CG/JU
Sample : 01050-04MEDL 10X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4477MEDL

Quant Time: Jan 12 17:55:16 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Jan 05 03:34:47 2023
Response via : Initial Calibration

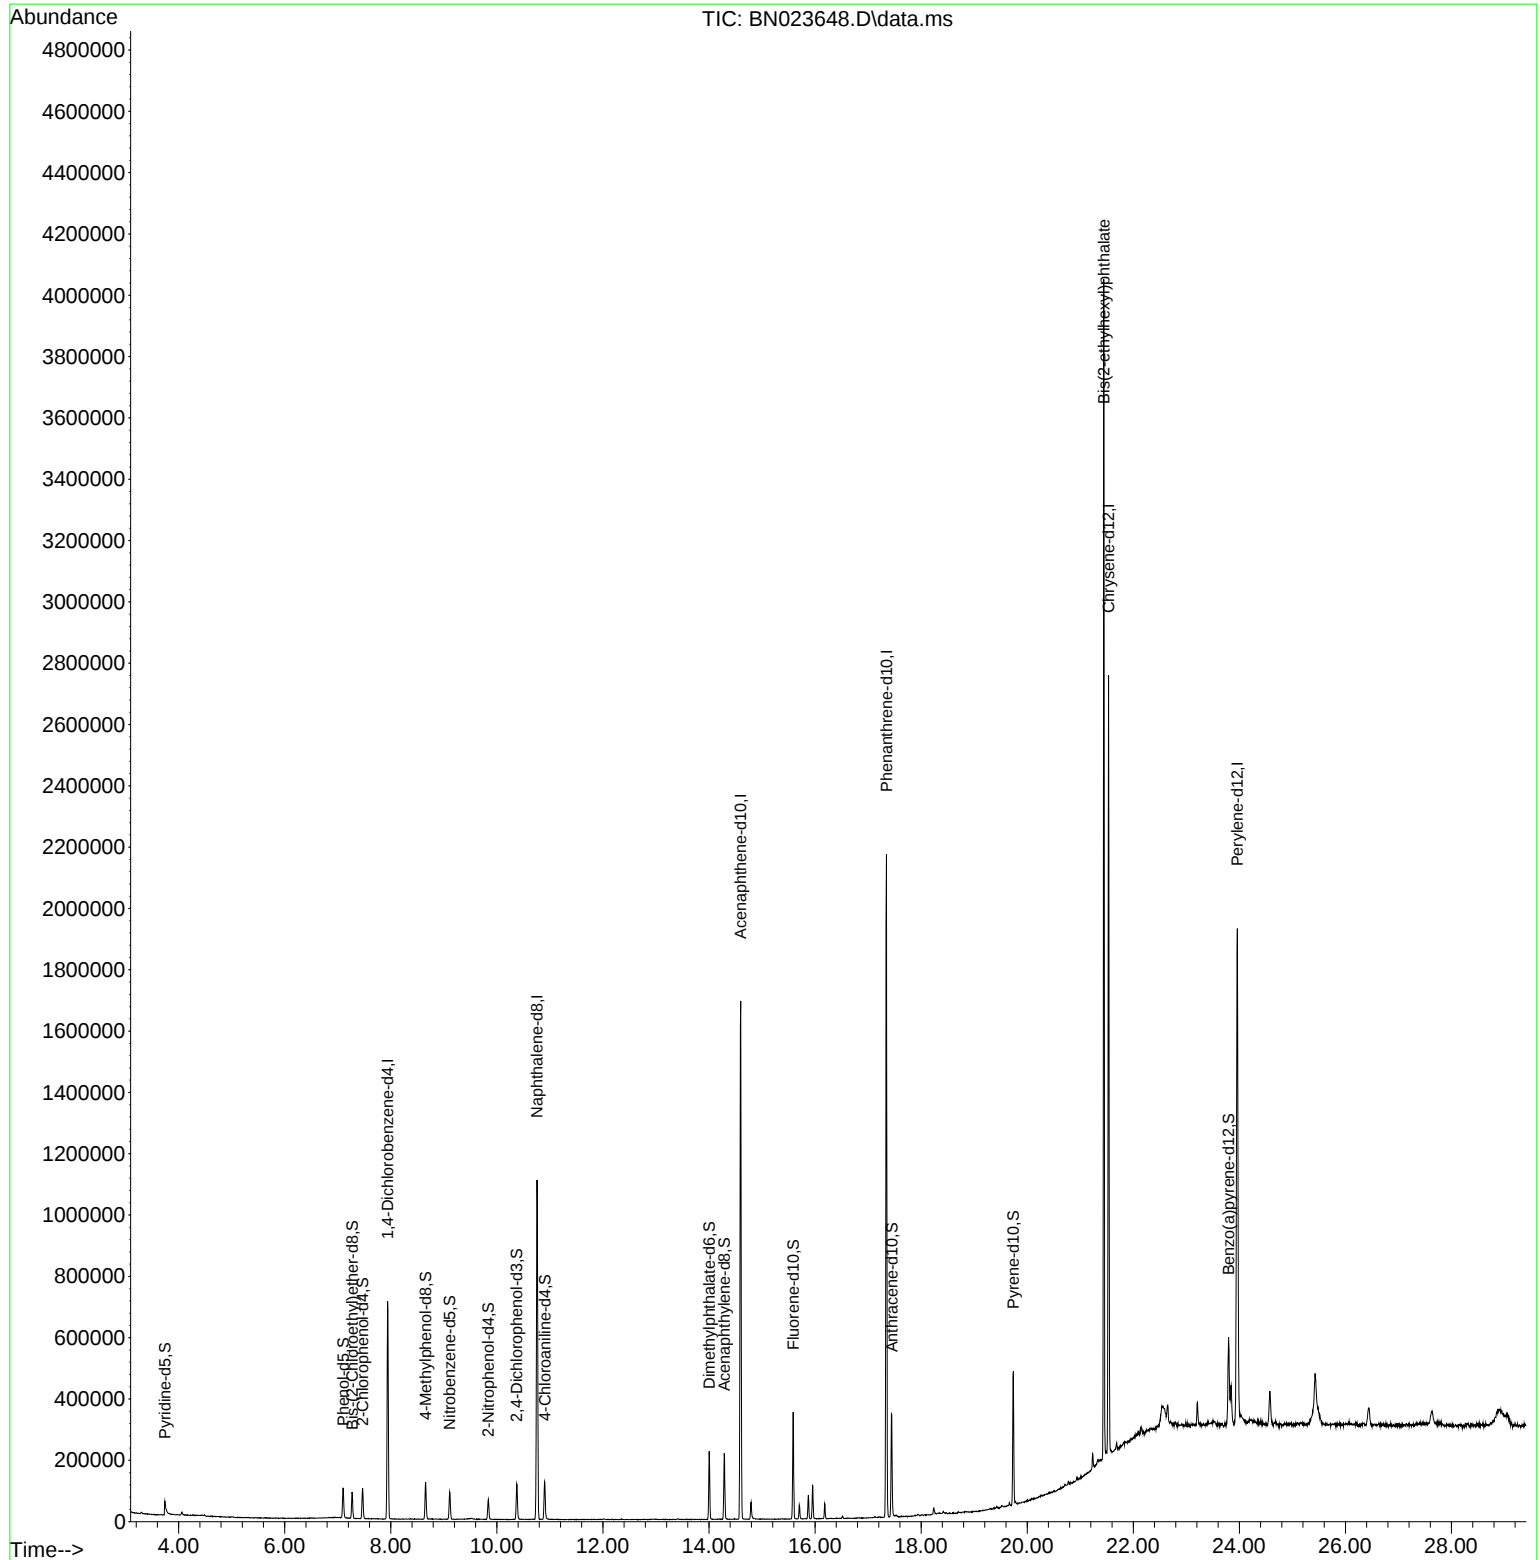

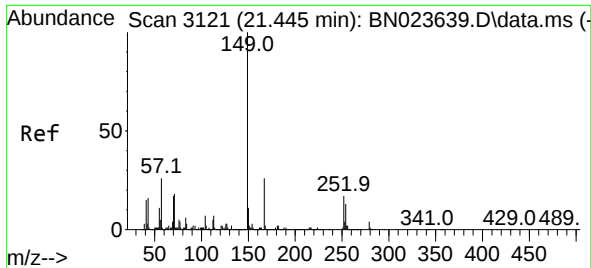

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 27.104 ng/ul
 RT: 21.445 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: BN023648.D
 Acq: 12 Jan 2023 17:24

Instrument :
 BNA_N
 ClientSampleId :
 A4477MEDL

Tgt Ion:149 Resp: 1170630
 Ion Ratio Lower Upper
 149 100
 167 26.7 22.0 33.0
 279 3.6 3.4 5.2

