

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
 Data File : BN023640.D
 Acq On : 12 Jan 2023 12:12
 Operator : CG/JU
 Sample : PB150090BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK090

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023640.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	43	rBV	38365	55088	1.26%	0.117%
2	3.723	105	108	132	rBV	511273	854191	19.60%	1.819%
3	4.058	162	165	174	rVB	11704	20260	0.46%	0.043%
4	7.105	676	683	694	rVB	751902	1150964	26.41%	2.451%
5	7.269	705	711	720	rVB	594144	919679	21.10%	1.959%
6	7.469	737	745	754	rBV	761813	1176980	27.01%	2.507%
7	7.940	818	825	834	rBV	667139	1061673	24.36%	2.261%
8	8.658	940	947	958	rBV	932588	1437067	32.97%	3.060%
9	9.116	1017	1025	1035	rBV	717071	1145934	26.29%	2.440%
10	9.840	1141	1148	1156	rBV	605584	944710	21.68%	2.012%
11	10.375	1232	1239	1252	rBV	937785	1496516	34.34%	3.187%
12	10.757	1296	1304	1313	rVB	1041216	1700415	39.02%	3.621%
13	10.899	1322	1328	1337	rBV	958726	1574869	36.14%	3.354%
14	12.351	1569	1575	1580	rBV	15089	24746	0.57%	0.053%
15	14.010	1850	1857	1864	rBV	1628646	2139451	49.09%	4.556%
16	14.293	1898	1905	1914	rBV	1854746	2596331	59.58%	5.529%
17	14.598	1950	1957	1965	rVB	1600076	2267345	52.03%	4.829%
18	14.793	1983	1990	2007	rVB	863331	1152966	26.46%	2.455%
19	15.587	2117	2125	2132	rBV	2383148	3292823	75.56%	7.013%
20	15.704	2139	2145	2157	rBV	706893	958129	21.99%	2.041%
21	15.828	2162	2166	2171	rVB2	10263	14354	0.33%	0.031%
22	17.134	2382	2388	2391	rVB3	3817	5660	0.13%	0.012%
23	17.345	2418	2424	2431	rBV	2005126	2777465	63.73%	5.915%
24	17.445	2434	2441	2453	rBV	2658936	3627718	83.24%	7.726%
25	18.251	2574	2578	2582	rVB6	3178	4473	0.10%	0.010%
26	19.304	2753	2757	2763	rVB2	30974	39657	0.91%	0.084%
27	19.369	2765	2768	2773	rVV	24409	32552	0.75%	0.069%
28	19.739	2825	2831	2840	rBV	3395917	4358078	100.00%	9.281%
29	21.533	3131	3136	3143	rBV	2406066	2979113	68.36%	6.345%
30	23.804	3514	3522	3537	rVB2	2122028	4233181	97.13%	9.015%
31	23.957	3542	3548	3557	rVB2	1450921	2913035	66.84%	6.204%




Sum of corrected areas: 46955423

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023640.D
Acq On : 12 Jan 2023 12:12
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

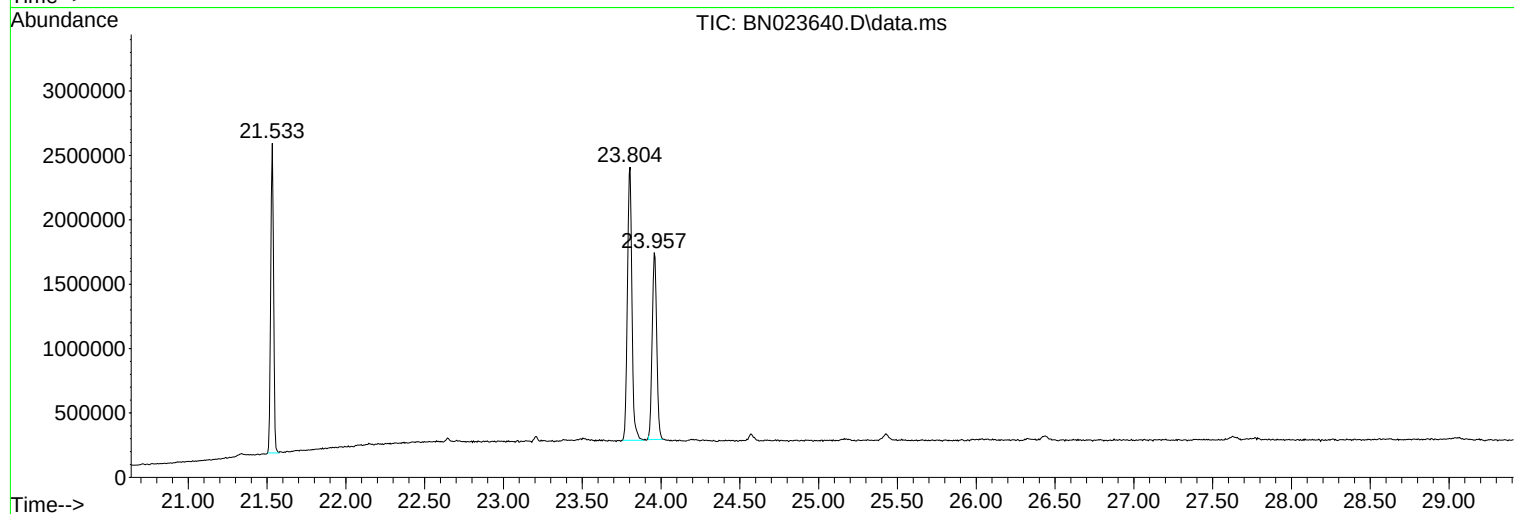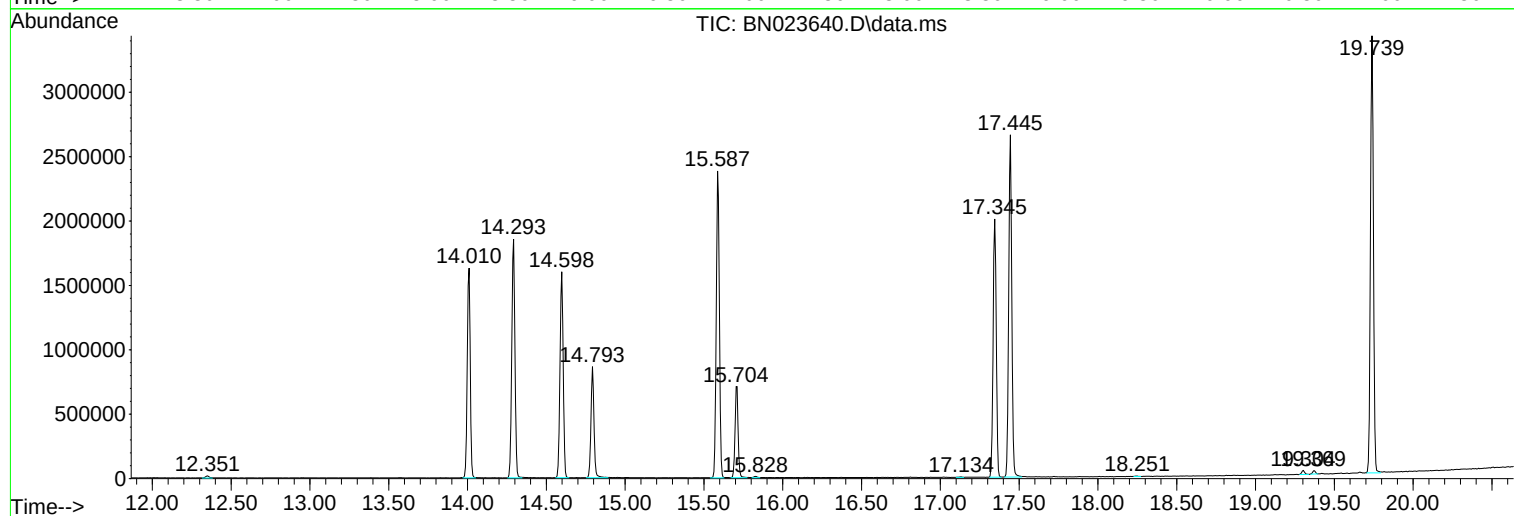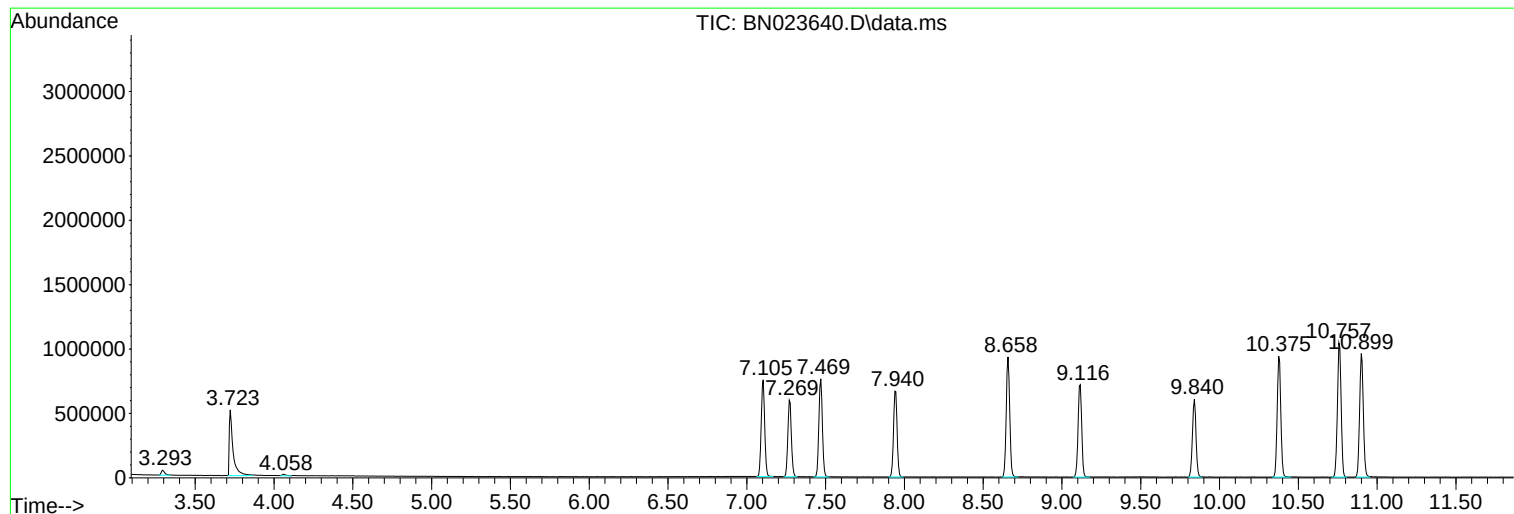

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023640.D
Acq On : 12 Jan 2023 12:12
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023640.D
Acq On : 12 Jan 2023 12:12
Operator : CG/JU
Sample : PB150090BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK090

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc