

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
 Data File : BN023642.D
 Acq On : 12 Jan 2023 13:26
 Operator : CG/JU
 Sample : PB150093BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK093

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023642.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	42	rVB	40069	55670	1.26%	0.120%
2	3.723	105	108	132	rBV	527144	890248	20.17%	1.922%
3	4.064	161	166	169	rBV2	10211	15202	0.34%	0.033%
4	7.105	676	683	692	rBV	758185	1165816	26.41%	2.517%
5	7.269	704	711	723	rBV	611390	936050	21.21%	2.021%
6	7.469	738	745	755	rBV	773059	1189954	26.96%	2.569%
7	7.940	818	825	833	rBV	601642	946763	21.45%	2.044%
8	8.658	940	947	957	rBV	945903	1459359	33.06%	3.151%
9	9.110	1016	1024	1035	rBV	715508	1152879	26.12%	2.489%
10	9.840	1141	1148	1160	rBV	614295	964764	21.86%	2.083%
11	10.375	1232	1239	1249	rBV	940132	1523996	34.53%	3.290%
12	10.757	1297	1304	1312	rVB	927834	1523821	34.53%	3.290%
13	10.899	1321	1328	1339	rBV	998622	1609131	36.46%	3.474%
14	12.346	1568	1574	1580	rVB2	15283	25022	0.57%	0.054%
15	14.004	1850	1856	1865	rBV	1572135	2182996	49.46%	4.713%
16	14.293	1897	1905	1917	rBV	1839691	2674273	60.59%	5.774%
17	14.598	1950	1957	1966	rVB	1426581	2060520	46.69%	4.449%
18	14.793	1983	1990	2003	rBV	861087	1176017	26.64%	2.539%
19	15.587	2118	2125	2132	rBV	2403323	3371709	76.39%	7.280%
20	15.704	2139	2145	2158	rBV	763843	995119	22.55%	2.149%
21	15.828	2162	2166	2170	rVB	11317	14052	0.32%	0.030%
22	17.345	2417	2424	2432	rBV	1728301	2464086	55.83%	5.320%
23	17.445	2434	2441	2453	rBV2	2634525	3713751	84.14%	8.018%
24	19.304	2753	2757	2762	rVB3	30913	40282	0.91%	0.087%
25	19.369	2764	2768	2773	rBV2	29332	44286	1.00%	0.096%
26	19.739	2825	2831	2846	rBV	3429708	4383347	99.31%	9.464%
27	21.533	3131	3136	3142	rBV	2195664	2648243	60.00%	5.718%
28	23.804	3514	3522	3535	rVB	2211672	4413655	100.00%	9.529%
29	23.957	3541	3548	3560	rVB2	1360181	2675688	60.62%	5.777%




Sum of corrected areas: 46316699

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023642.D
Acq On : 12 Jan 2023 13:26
Operator : CG/JU
Sample : PB150093BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

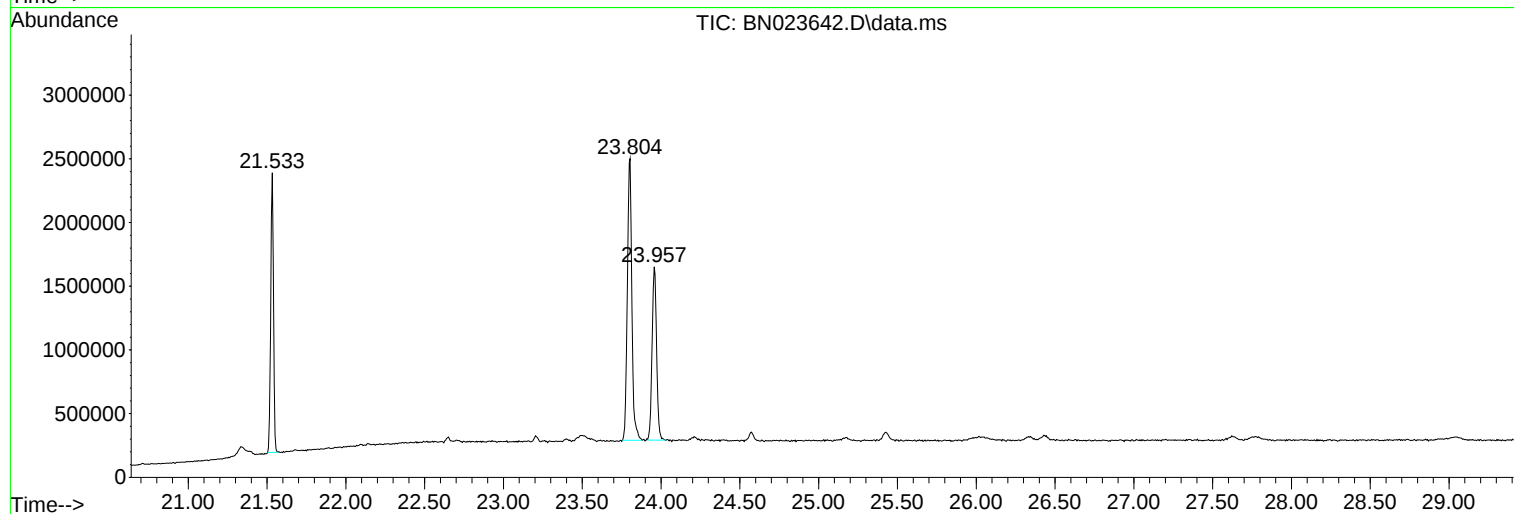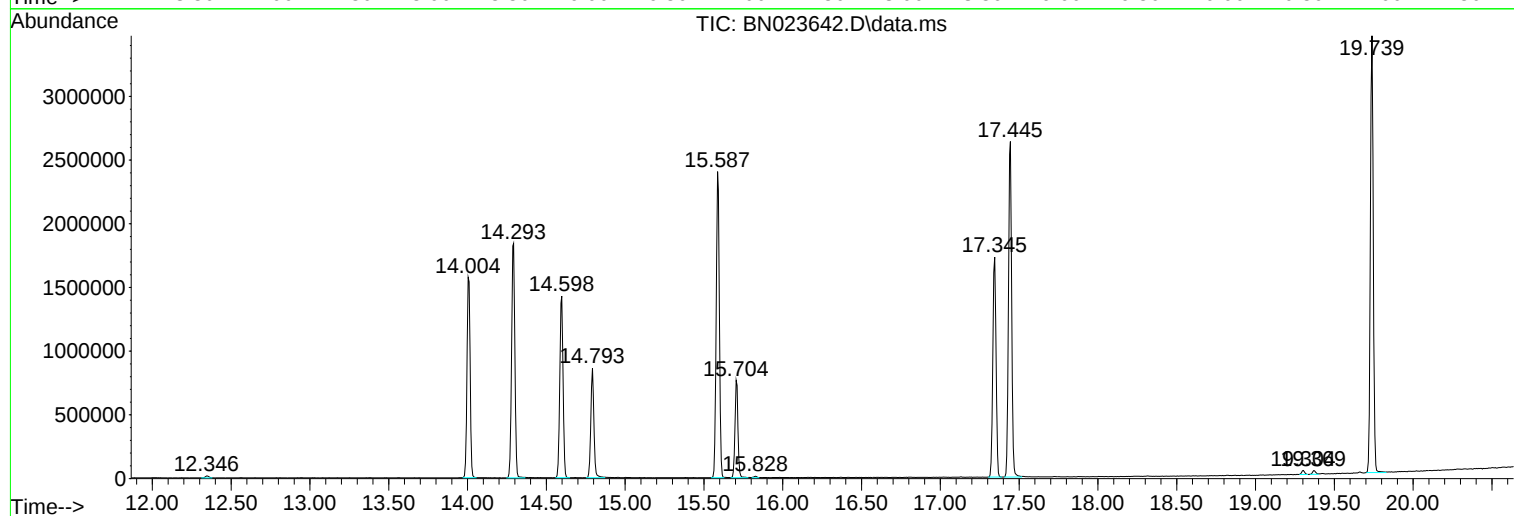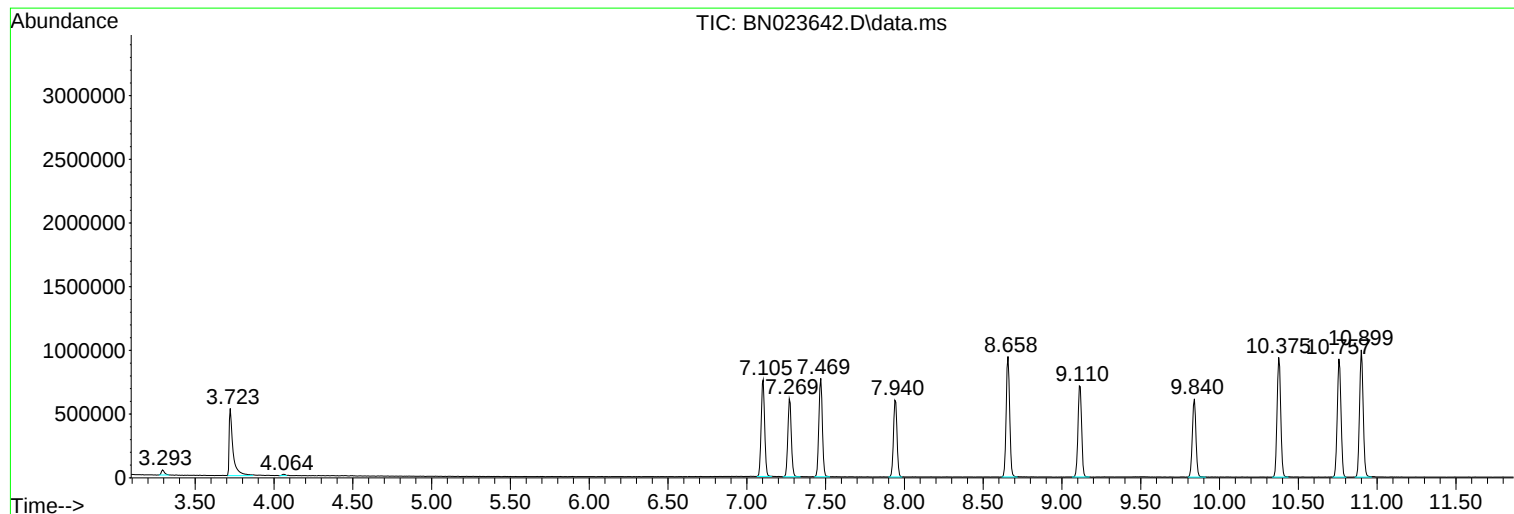

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023642.D
Acq On : 12 Jan 2023 13:26
Operator : CG/JU
Sample : PB150093BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023642.D
Acq On : 12 Jan 2023 13:26
Operator : CG/JU
Sample : PB150093BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK093

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc