

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
 Data File : BN023644.D
 Acq On : 12 Jan 2023 14:39
 Operator : CG/JU
 Sample : PB150092BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK092

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
 Title : SVOA CALIBRATION

Signal : TIC: BN023644.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	31	35	45	rVB	43170	64798	1.37%	0.133%
2	3.722	105	108	132	rBV	550786	918754	19.49%	1.891%
3	4.058	162	165	171	rVB2	10220	14991	0.32%	0.031%
4	7.105	675	683	699	rVB	789954	1230348	26.10%	2.532%
5	7.269	705	711	723	rVB	631099	973079	20.64%	2.003%
6	7.469	738	745	755	rVB	816390	1245556	26.43%	2.564%
7	7.940	818	825	832	rBV	625601	985526	20.91%	2.028%
8	8.657	939	947	960	rBV	1003217	1525783	32.37%	3.140%
9	9.110	1017	1024	1032	rBV	769017	1208224	25.63%	2.487%
10	9.840	1139	1148	1159	rBV	630010	1009616	21.42%	2.078%
11	10.375	1232	1239	1251	rBV	984515	1564651	33.20%	3.220%
12	10.757	1297	1304	1312	rBV	971986	1581293	33.55%	3.255%
13	10.899	1321	1328	1339	rBV	1020425	1670199	35.43%	3.438%
14	12.346	1569	1574	1581	rBV2	16226	25316	0.54%	0.052%
15	14.010	1850	1857	1870	rVB	1695405	2312577	49.06%	4.760%
16	14.292	1898	1905	1913	rBV	1931277	2756065	58.47%	5.672%
17	14.598	1950	1957	1964	rBV	1535006	2145779	45.52%	4.416%
18	14.792	1984	1990	2004	rBV	921504	1231072	26.12%	2.534%
19	15.587	2118	2125	2132	rBV	2565658	3503560	74.33%	7.211%
20	15.704	2139	2145	2159	rBV	804434	1059560	22.48%	2.181%
21	15.828	2162	2166	2171	rVB4	10979	15074	0.32%	0.031%
22	17.134	2384	2388	2393	rBV4	3486	4865	0.10%	0.010%
23	17.345	2418	2424	2430	rBV	1914850	2560377	54.32%	5.270%
24	17.445	2434	2441	2456	rBV	2822970	3832161	81.30%	7.887%
25	19.304	2753	2757	2762	rVB	30792	41742	0.89%	0.086%
26	19.369	2764	2768	2774	rVV	30345	42289	0.90%	0.087%
27	19.663	2816	2818	2821	rVB4	8144	7441	0.16%	0.015%
28	19.739	2825	2831	2838	rBV	3509869	4529090	96.09%	9.321%
29	21.533	3131	3136	3141	rBV2	2245807	2773598	58.84%	5.708%
30	23.804	3514	3522	3537	rBV	2336964	4713466	100.00%	9.701%
31	23.957	3542	3548	3558	rVB2	1438083	2774479	58.86%	5.710%
32	24.574	3650	3653	3662	rVB	142188	266248	5.65%	0.548%




Sum of corrected areas: 48587577

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023644.D
Acq On : 12 Jan 2023 14:39
Operator : CG/JU
Sample : PB150092BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

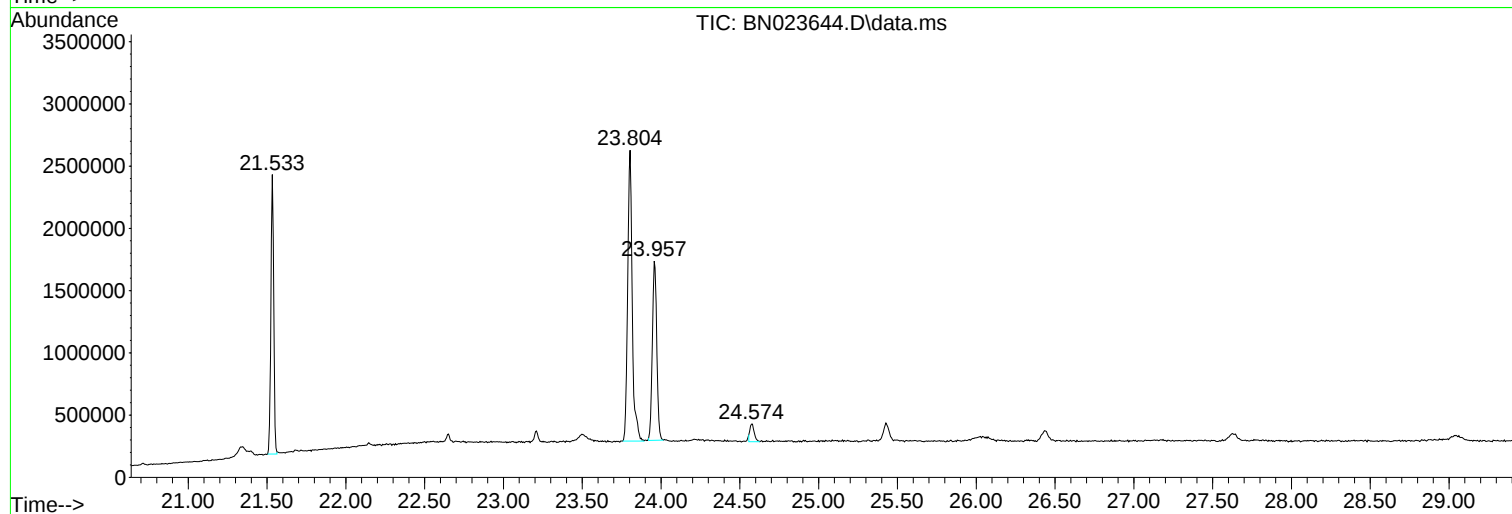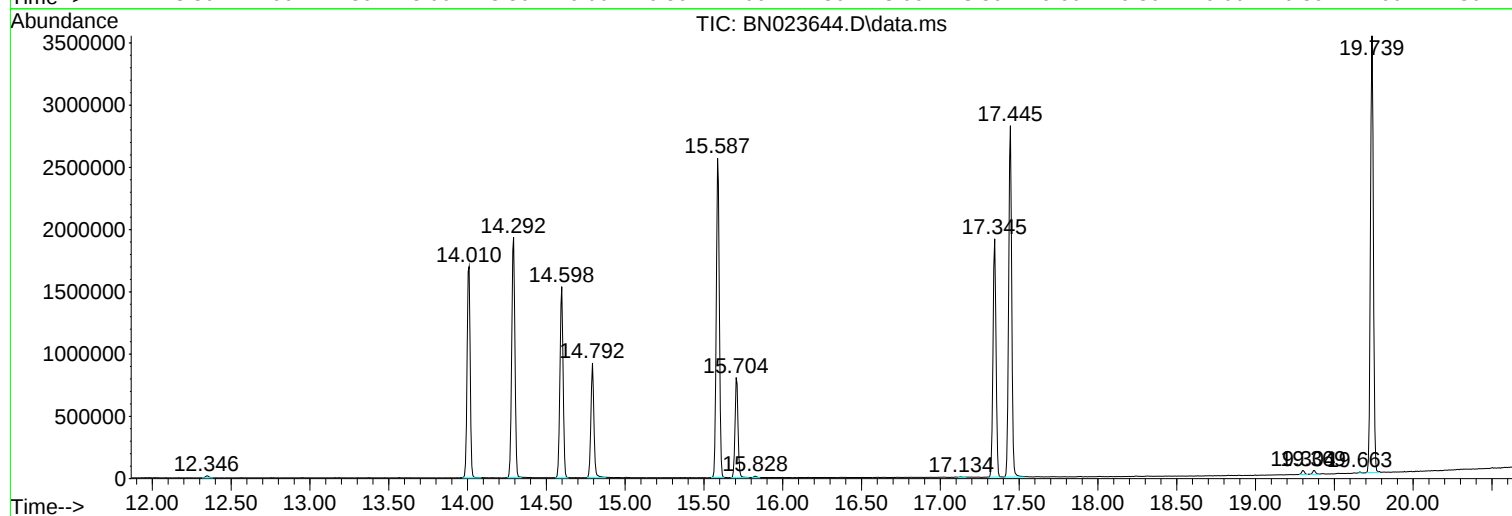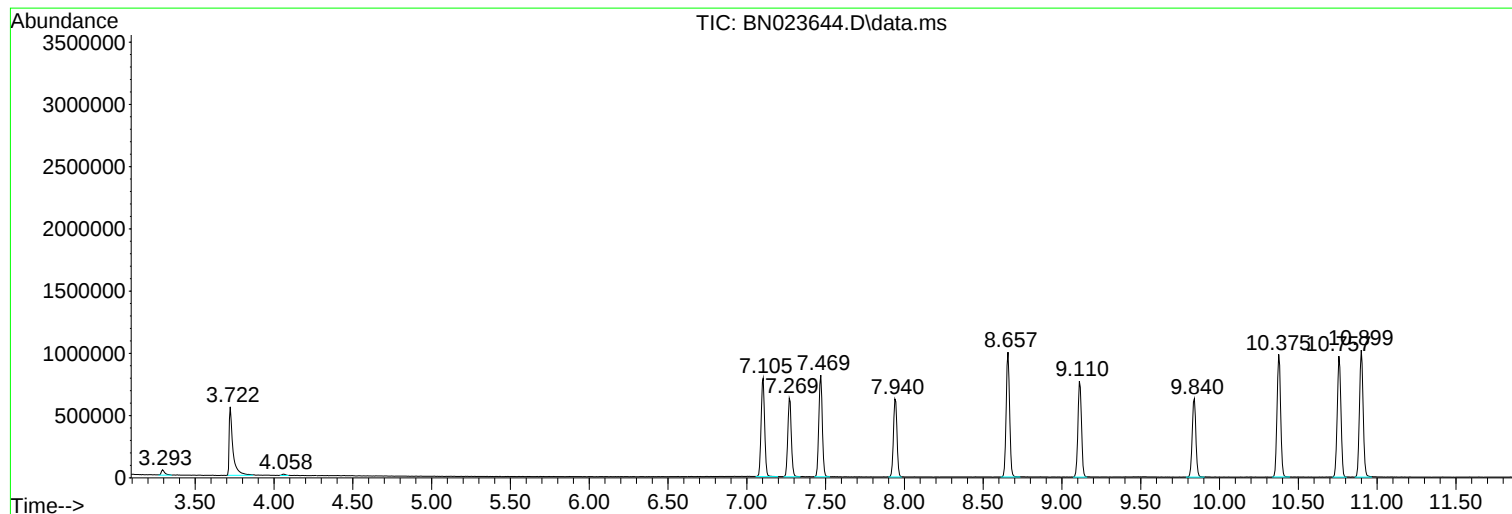

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023644.D
Acq On : 12 Jan 2023 14:39
Operator : CG/JU
Sample : PB150092BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011323\
Data File : BN023644.D
Acq On : 12 Jan 2023 14:39
Operator : CG/JU
Sample : PB150092BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK092

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN010523.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc