


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN011420\
 Data File : BN009362.D
 Acq On : 13 Jan 2020 13:54
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

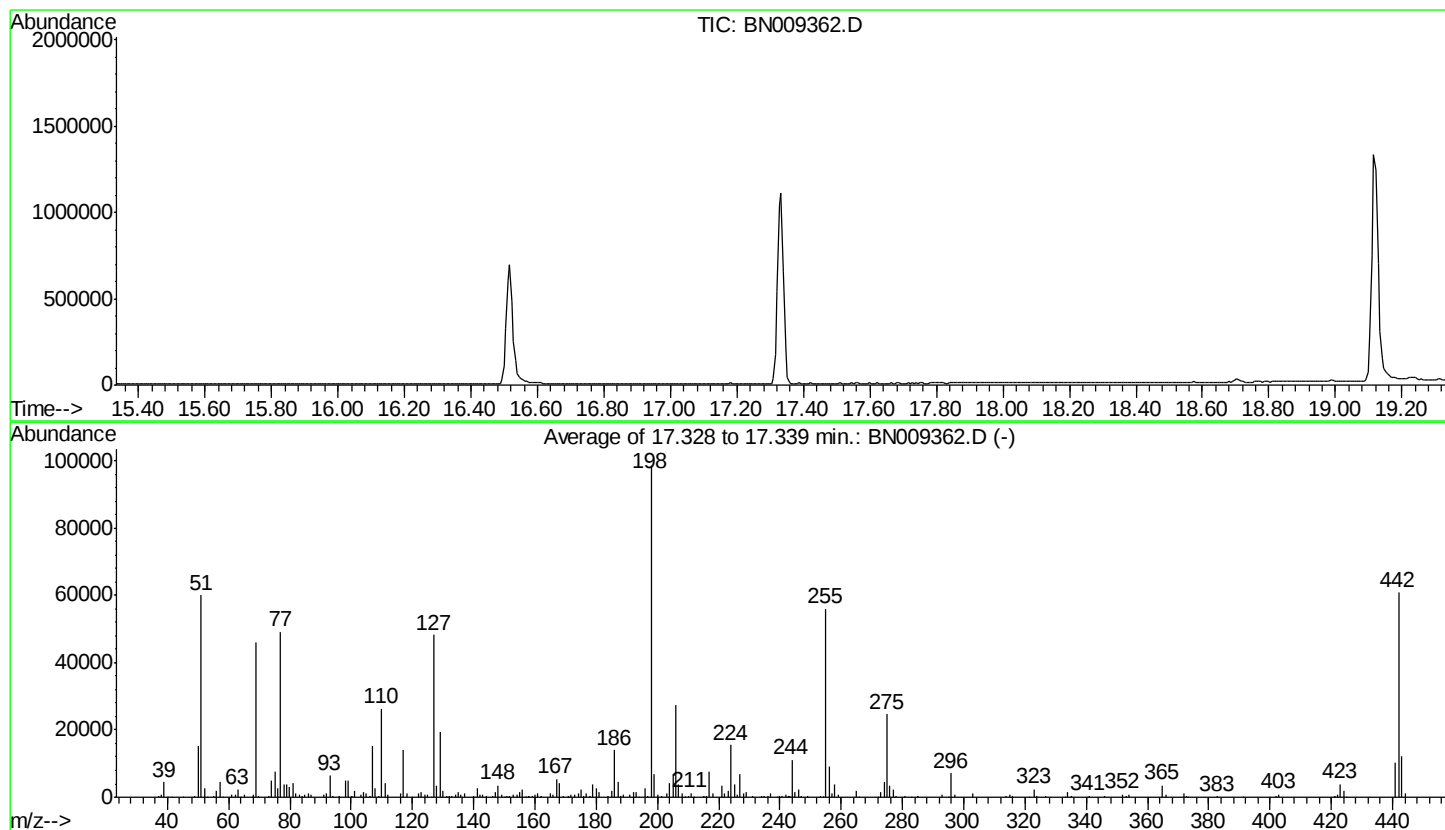

AutoFind: Scans 2438, 2439, 2440; Background Corrected with Scan 2432

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.9	60016	PASS
68	69	0.00	2	1.6	723	PASS
69	198	0.00	100	46.6	45882	PASS
70	69	0.00	2	0.5	221	PASS
127	198	10	80	48.9	48154	PASS
197	198	0.00	2	0.4	385	PASS
198	198	100	100	100.0	98554	PASS
199	198	5	9	7.0	6876	PASS
275	198	10	60	25.0	24608	PASS
365	198	1	100	3.6	3526	PASS
441	198	0.01	100	10.5	10314	PASS
442	198	50	100	61.7	60834	PASS
443	442	15	24	20.2	12315	PASS