
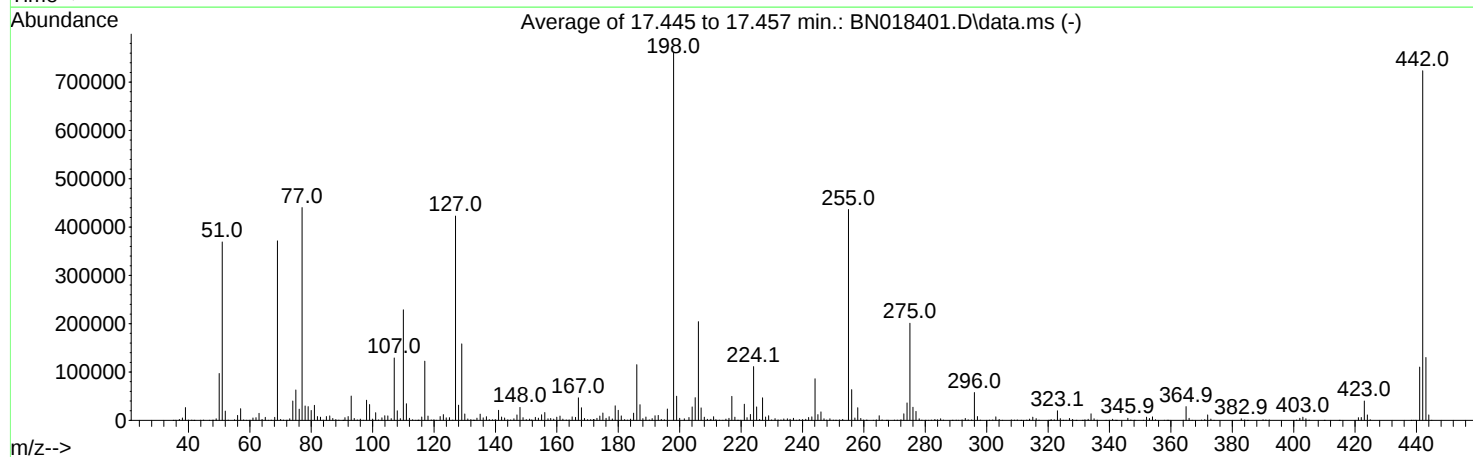


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011422\
 Data File : BN018401.D
 Acq On : 14 Jan 2022 09:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN010722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jan 14 12:12:13 2022

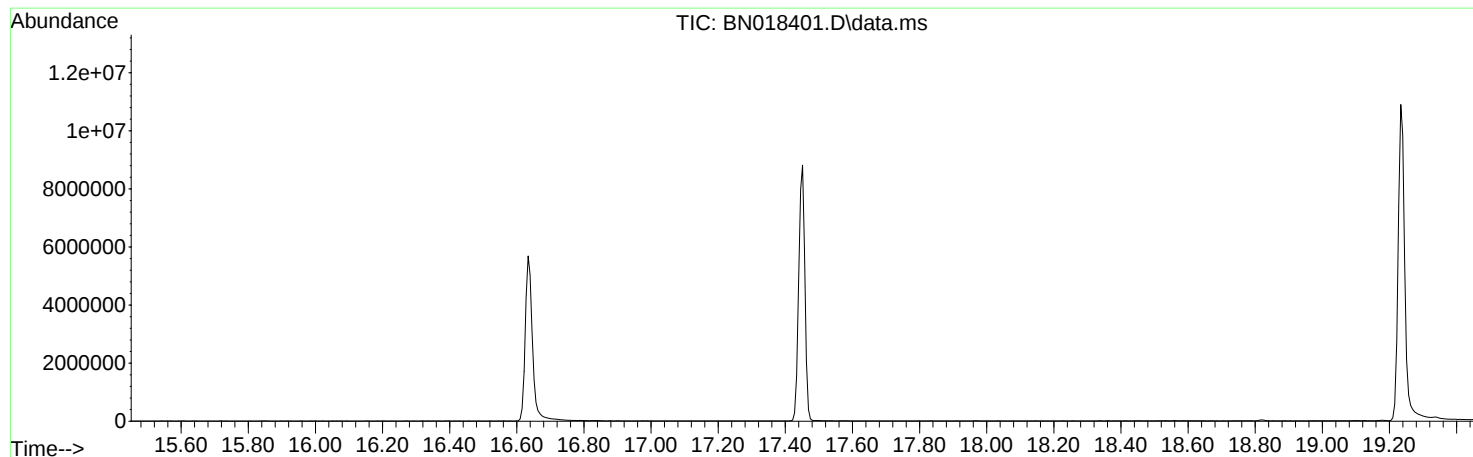




AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2450

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.5	369246	PASS
68	69	0.00	2	1.7	6318	PASS
69	198	0.00	100	48.8	371669	PASS
70	69	0.00	2	0.5	1926	PASS
127	198	10	80	55.6	422933	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	761301	PASS
199	198	5	9	6.6	50040	PASS
275	198	10	60	26.4	201024	PASS
365	198	1	100	3.7	28515	PASS
441	198	0.01	100	14.5	110397	PASS
442	442	50	100	100.0	723520	PASS
443	442	15	24	18.0	129992	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011422\
Data File : BN018401.D
Acq On : 14 Jan 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 14 12:23:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 12:23:46 2022
Response via : Initial Calibration

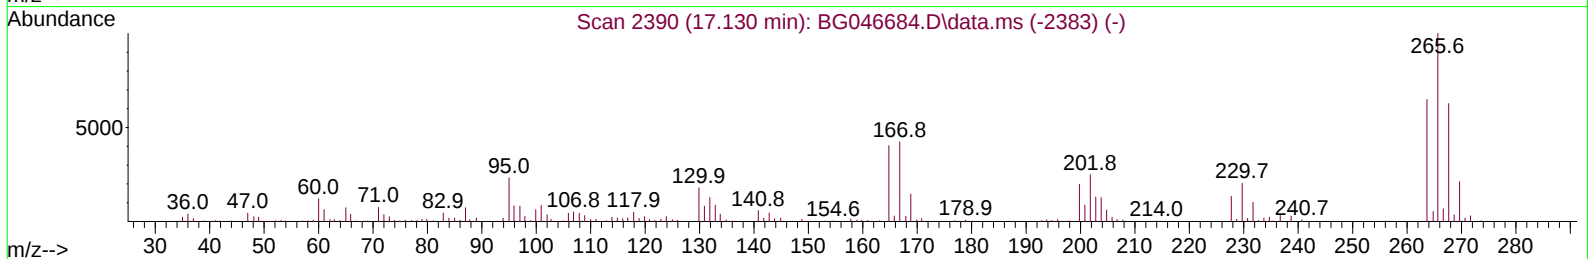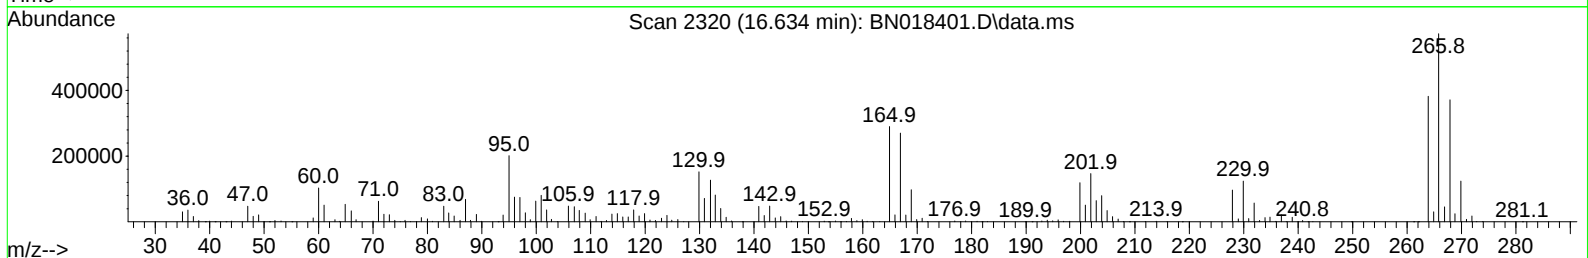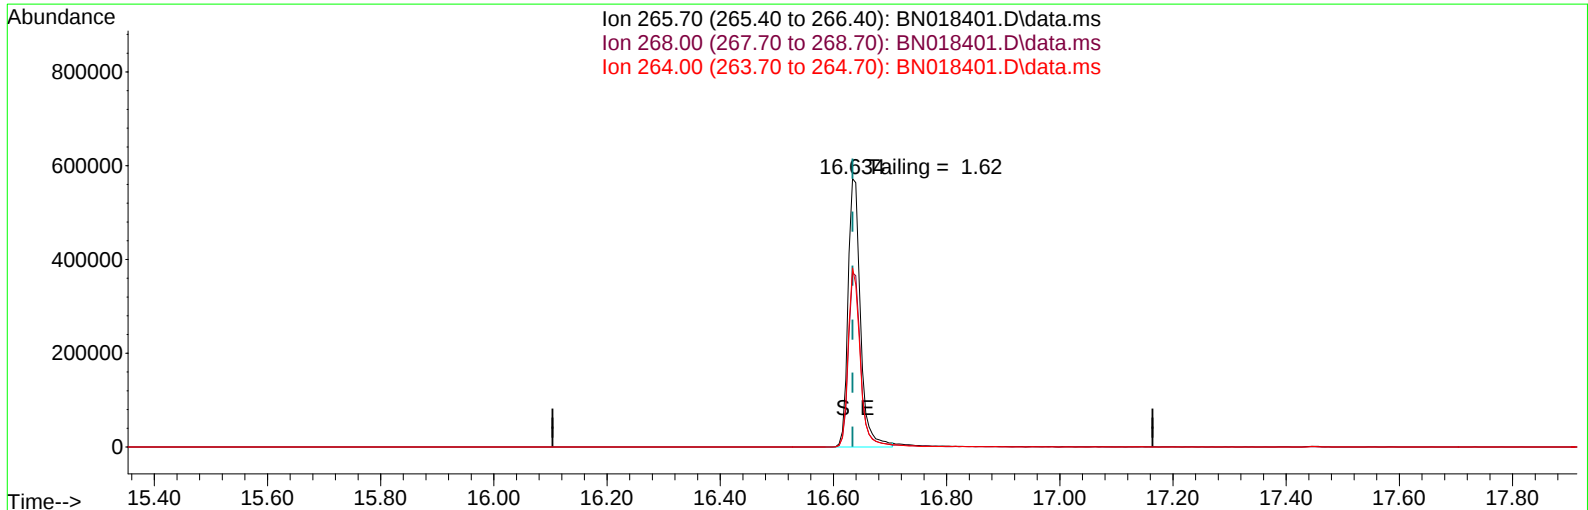

TIC: BN018401.D\data.ms

(70) Pentachlorophenol (C)

16.634min (0.000) 20179.14 ng




response 891413

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.88
264.00	61.60	66.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011422\
Data File : BN018401.D
Acq On : 14 Jan 2022 09:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 14 12:23:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jan 14 12:23:46 2022
Response via : Initial Calibration

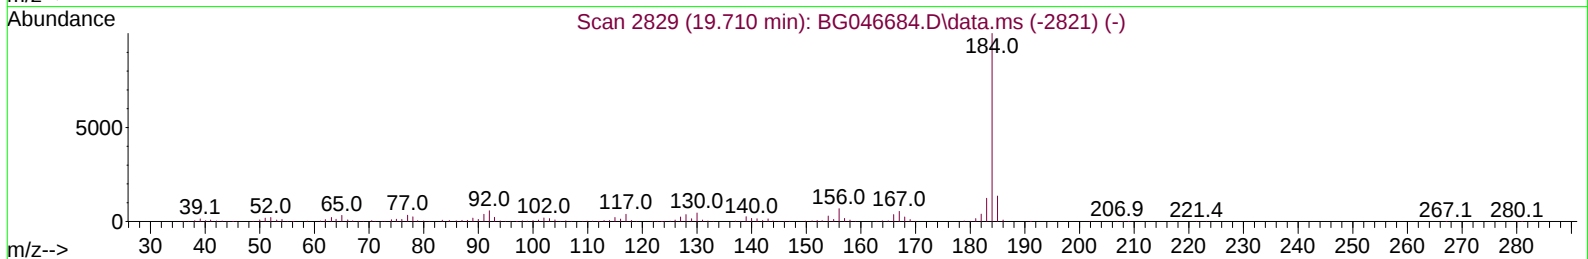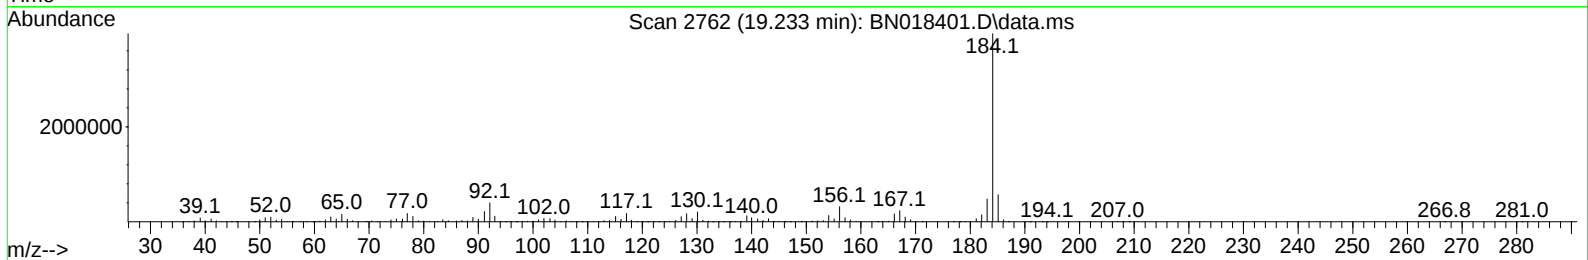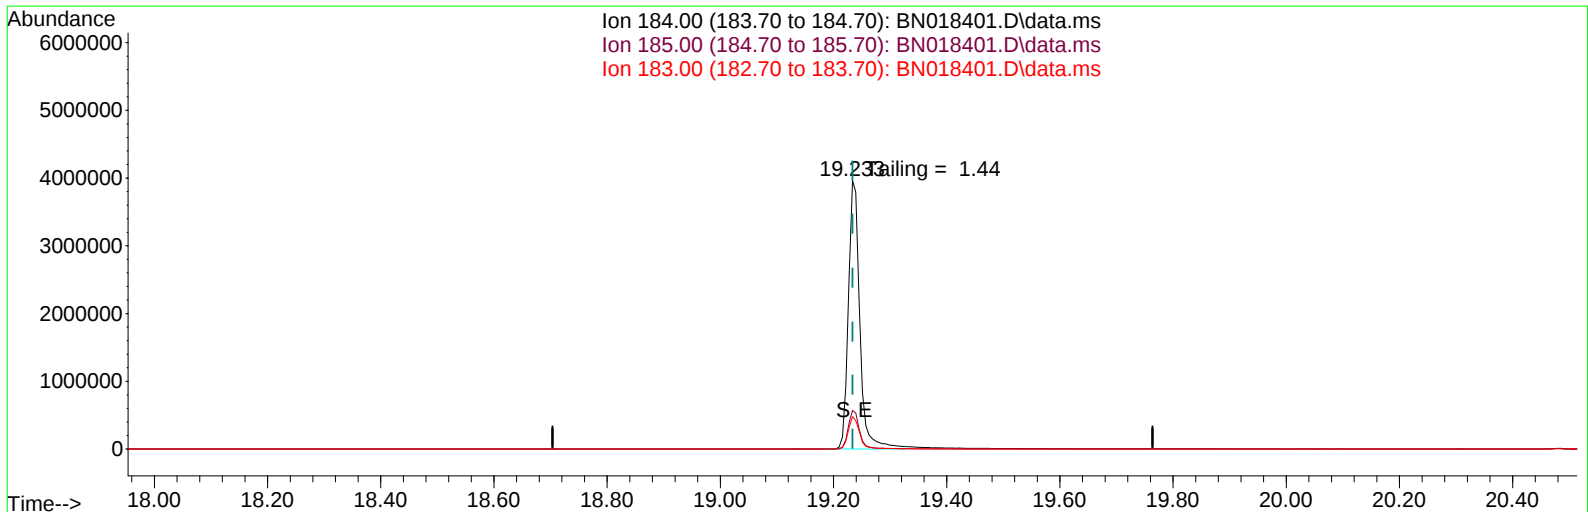

TIC: BN018401.D\data.ms

(77) Benzidine

19.233min (0.000) 0.00 ng

response 5720563

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.40
183.00	13.20	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/14/2022	BNA_N	<u>BN018401.D</u>
Compound Name	Response	Retention Time
DDT	2758072	20.48
DDD	20956	20.03
DDE	1391	19.53
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
22347	2780419	0.80

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP