
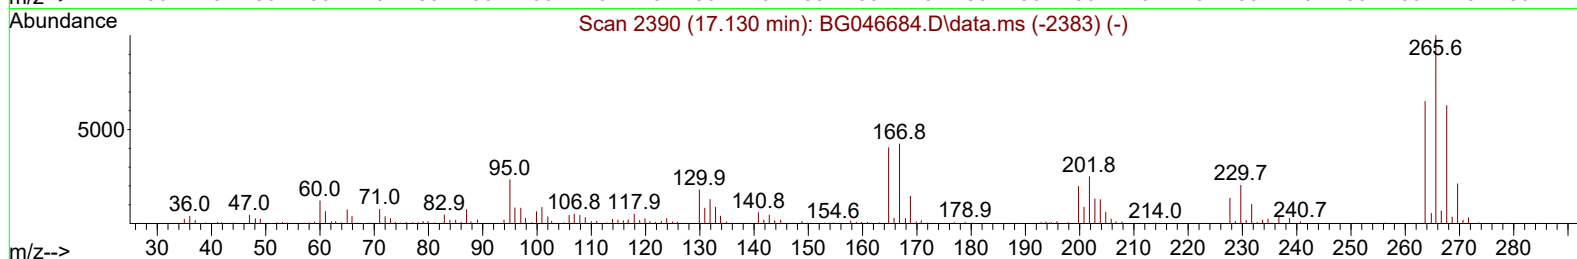
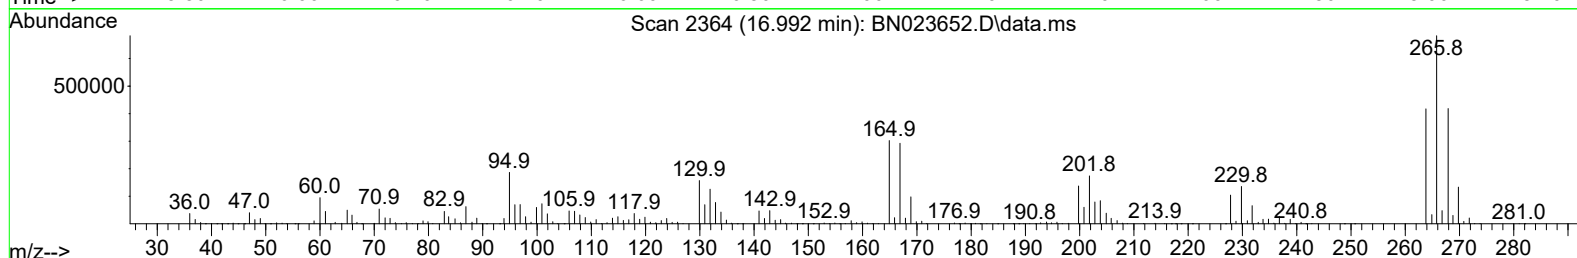


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011423\
Data File : BN023652.D
Acq On : 13 Jan 2023 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 03:12:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 16 03:11:56 2023
Response via : Initial Calibration

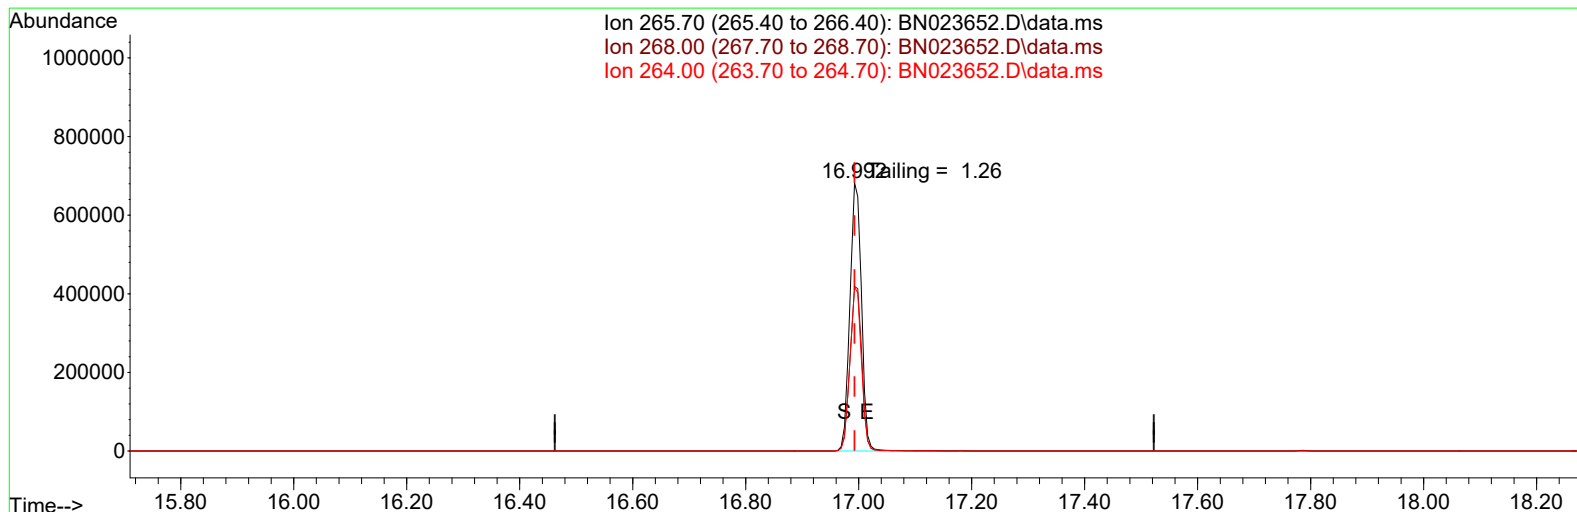

TIC: BN023652.D\data.ms

(70) Pentachlorophenol (C)




16.992min (0.000) 27529.85 ng

response 976102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.32
264.00	61.60	61.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011423\
 Data File : BN023652.D
 Acq On : 13 Jan 2023 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 16 03:12:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 16 03:11:56 2023
 Response via : Initial Calibration

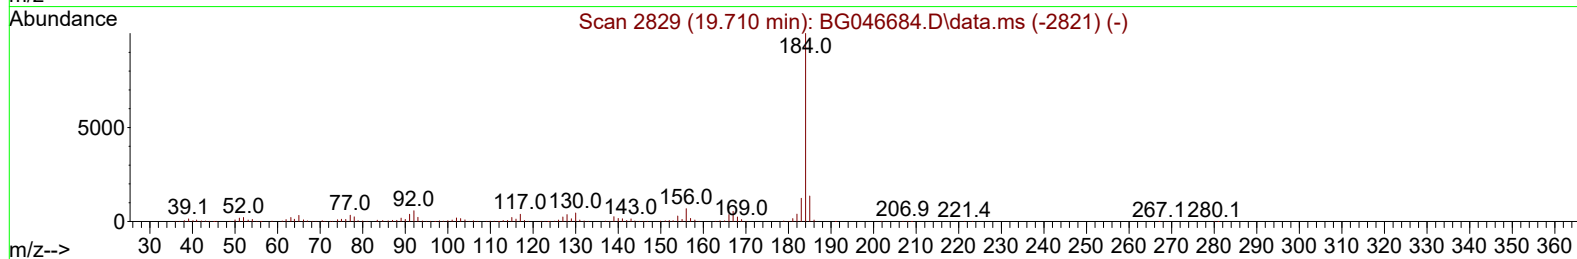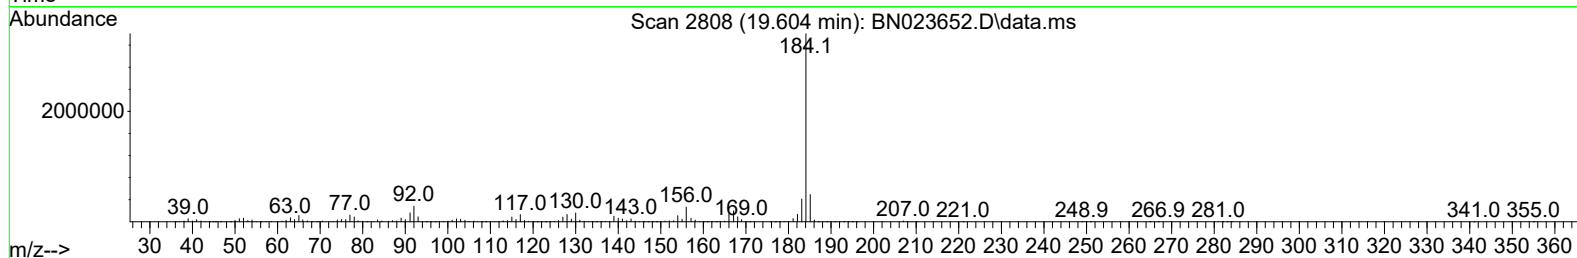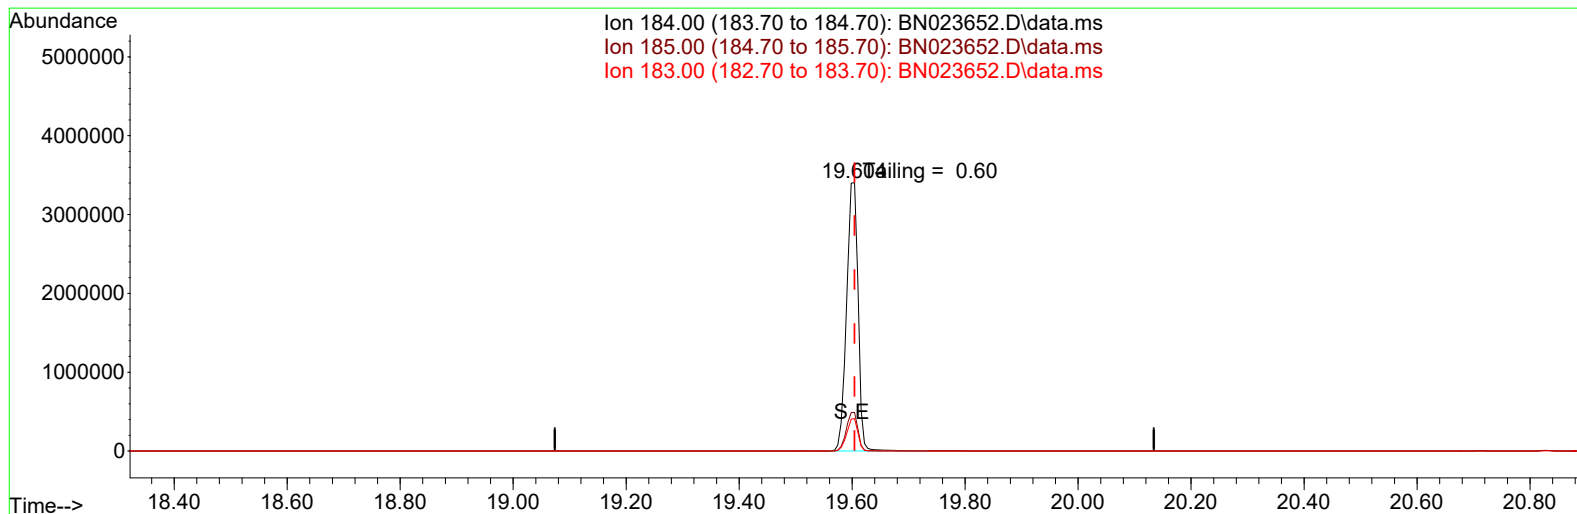

TIC: BN023652.D\data.ms

(77) Benzidine**19.604min (0.000) 811891.09 ng****response 4830181**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	12.11
0.00	0.00	0.00