
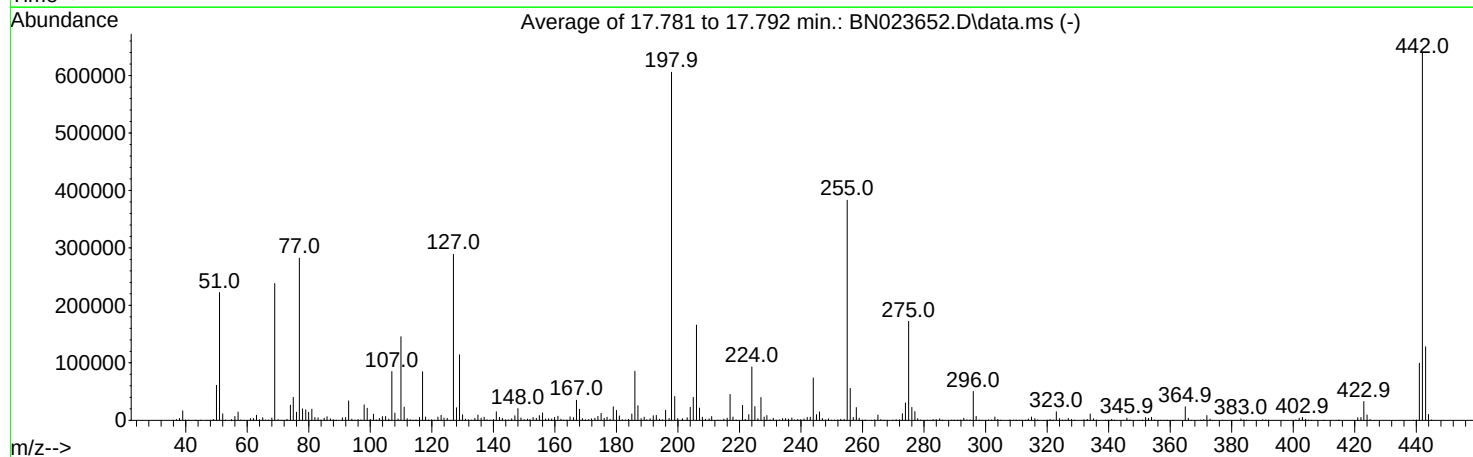


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011423\
 Data File : BN023652.D
 Acq On : 13 Jan 2023 12:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jan 12 00:22:07 2023

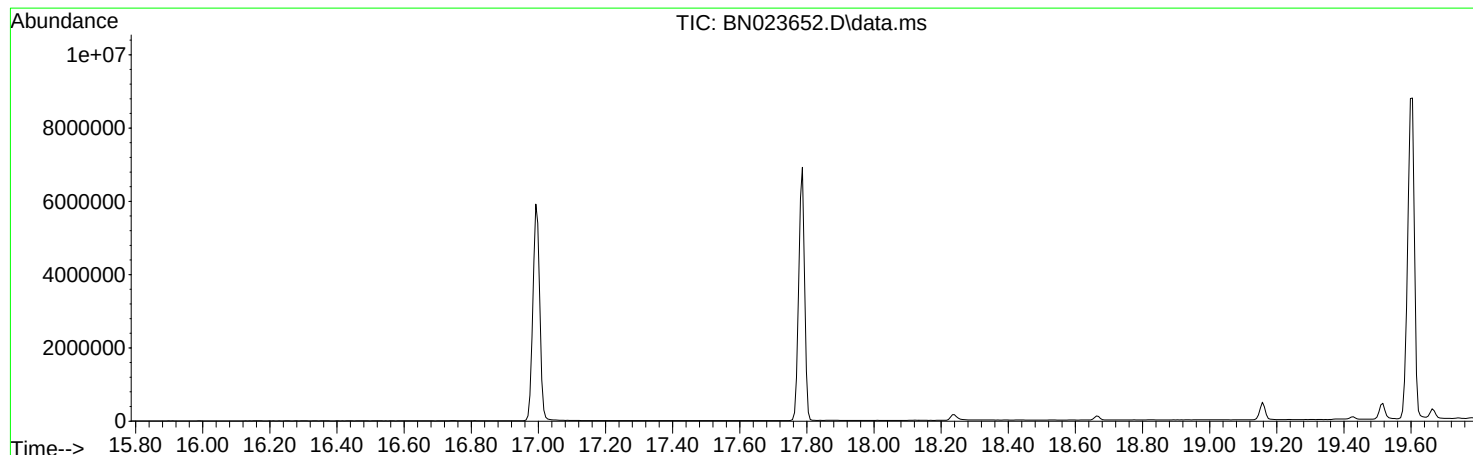




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2491

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	222329	PASS
68	69	0.00	2	1.7	4090	PASS
69	198	0.00	100	39.3	237952	PASS
70	69	0.00	2	0.6	1396	PASS
127	198	10	80	47.7	288981	PASS
197	198	0.00	2	0.5	3189	PASS
198	198	100	100	100.0	605867	PASS
199	198	5	9	6.8	41403	PASS
275	198	10	60	28.4	172181	PASS
365	198	1	100	3.9	23437	PASS
441	198	0.01	100	16.4	99269	PASS
442	442	50	100	100.0	640213	PASS
443	442	15	24	20.0	127864	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011423\
Data File : BN023652.D
Acq On : 13 Jan 2023 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 16 03:12:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 16 03:11:56 2023
Response via : Initial Calibration

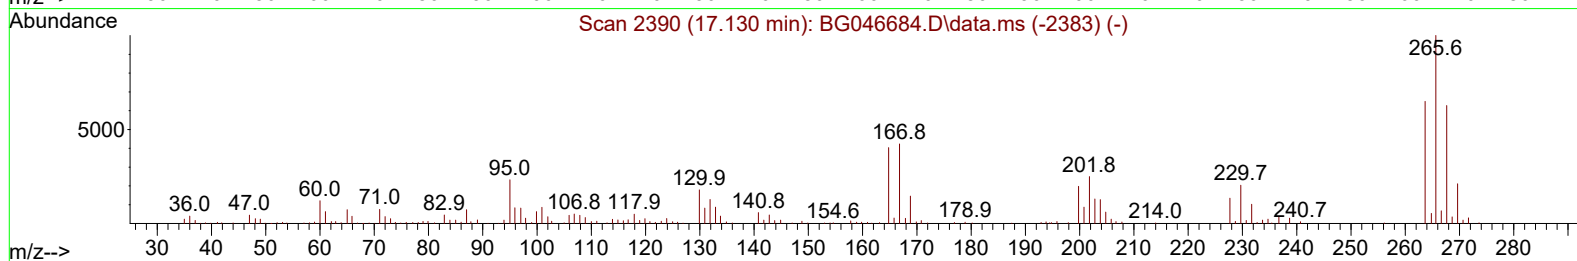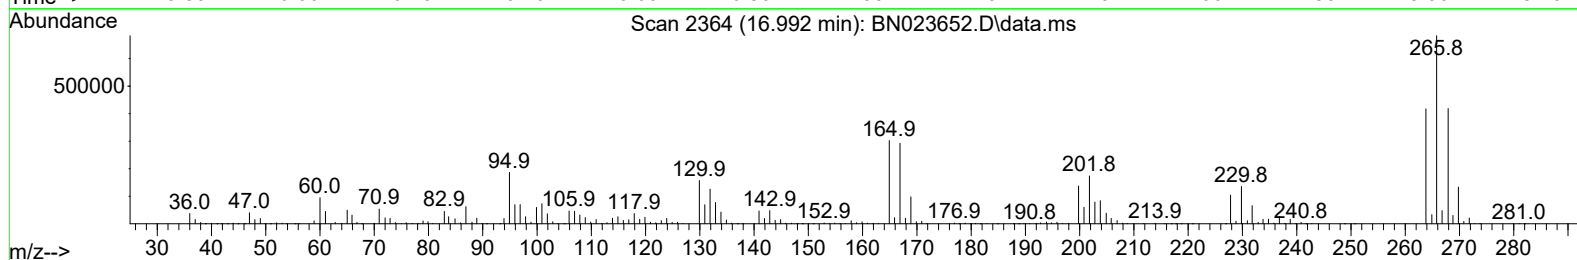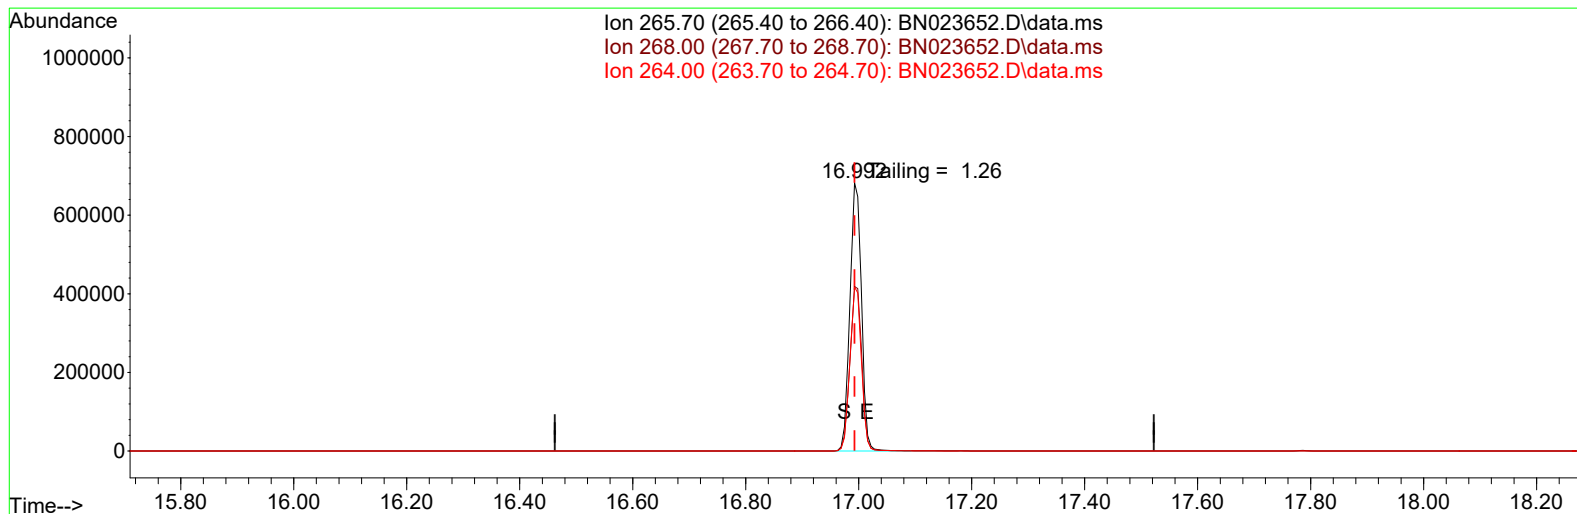

TIC: BN023652.D\data.ms

(70) Pentachlorophenol (C)

16.992min (0.000) 27529.85 ng




response 976102

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.32
264.00	61.60	61.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011423\
Data File : BN023652.D
Acq On : 13 Jan 2023 12:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 16 03:12:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 16 03:11:56 2023
Response via : Initial Calibration

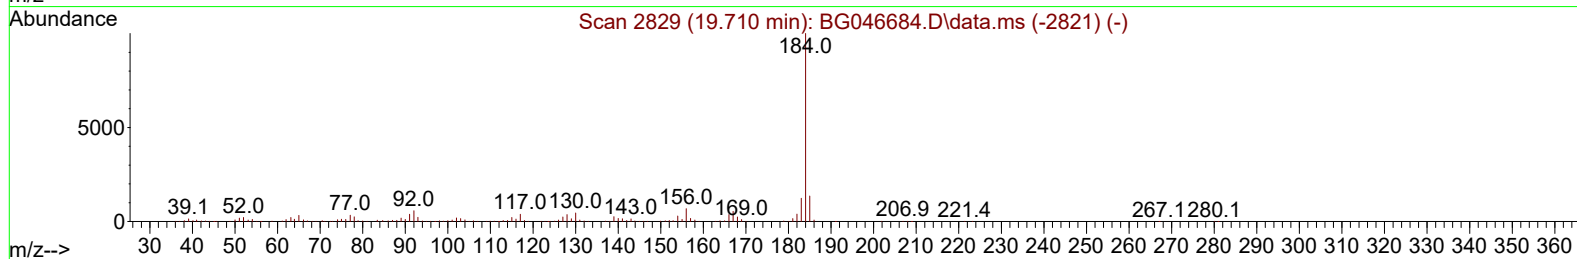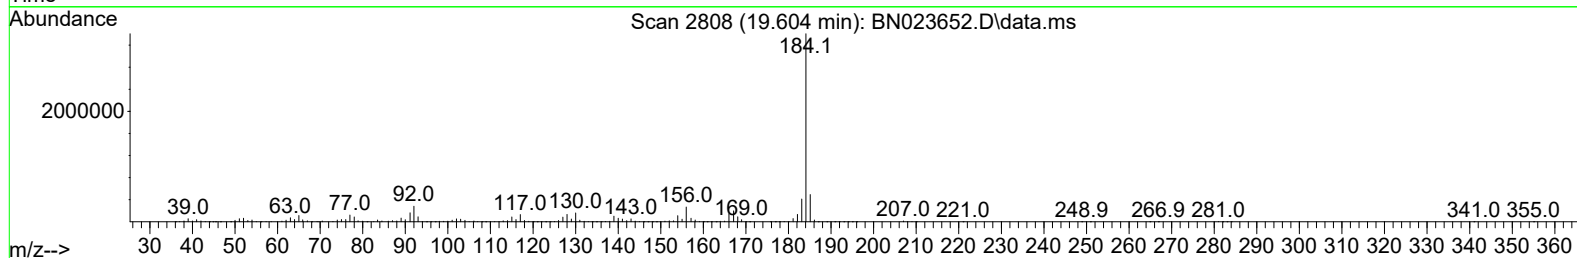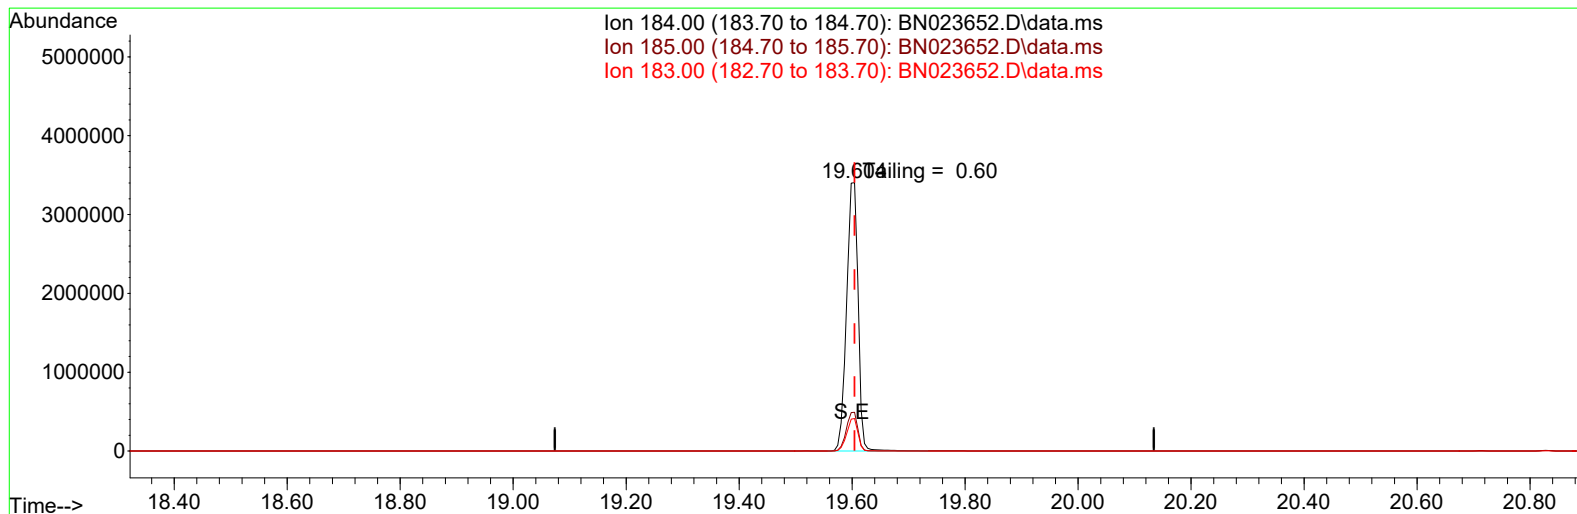

TIC: BN023652.D\data.ms

(77) Benzidine

19.604min (0.000) 811891.09 ng

response 4830181

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.46
183.00	13.20	12.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/14/2023	BNA_N	<u>BN023652.D</u>
Compound Name	Response	Retention Time
DDT	2339165	20.828
DDD	105343	20.386
DDE	2213	19.881
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
107556	2446721	4.40

Instrument :
BNA_N
ClientSampleId :
DFTPP