


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN011520\
 Data File : BN009371.D
 Acq On : 15 Jan 2020 09:45
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

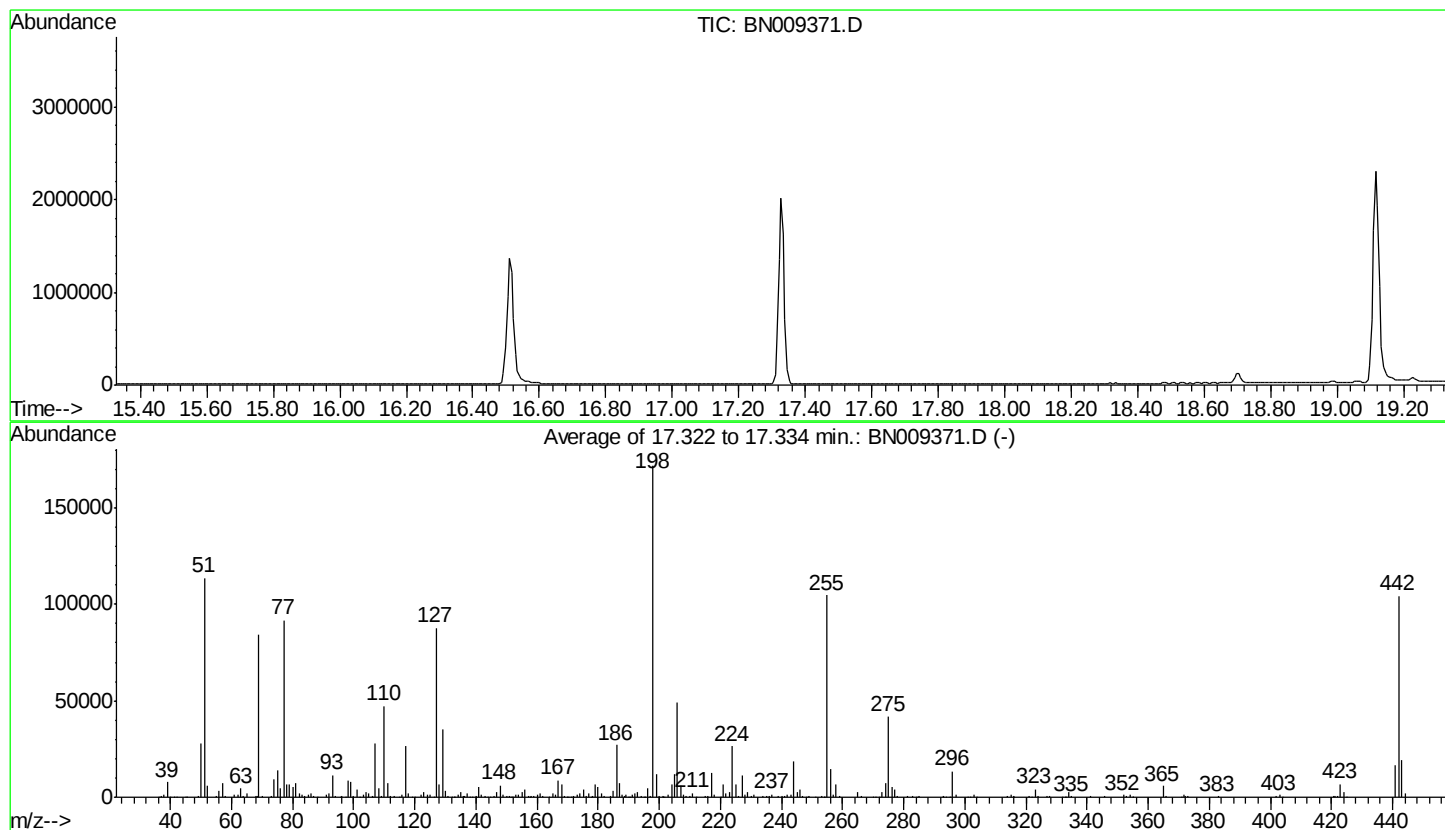

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	66.1	113560	PASS
68	69	0.00	2	1.1	899	PASS
69	198	0.00	100	48.9	84064	PASS
70	69	0.00	2	0.7	610	PASS
127	198	10	80	51.1	87904	PASS
197	198	0.00	2	0.3	532	PASS
198	198	100	100	100.0	171925	PASS
199	198	5	9	7.0	12070	PASS
275	198	10	60	24.3	41736	PASS
365	198	1	100	3.4	5827	PASS
441	198	0.01	100	9.6	16440	PASS
442	198	50	100	60.7	104282	PASS
443	442	15	24	18.2	18993	PASS