


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011525\
Data File : BN035925.D
Acq On : 15 Jan 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN010225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 02 15:39:17 2025

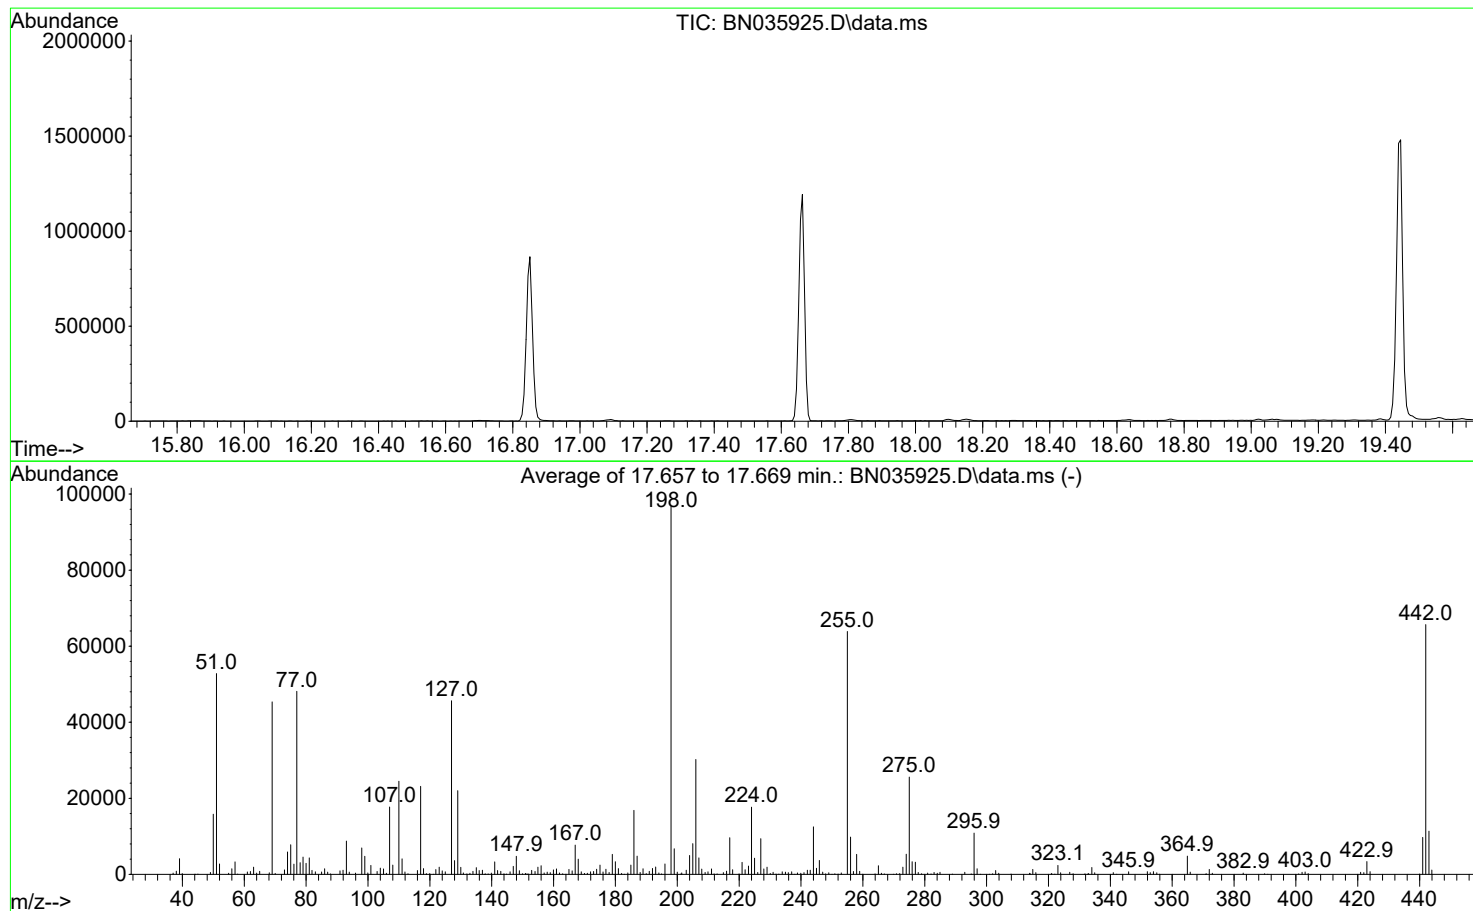

AutoFind: Scans 2460, 2461, 2462; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.6	52803	PASS
68	69	0.00	2	1.0	434	PASS
69	198	0.00	100	46.9	45360	PASS
70	69	0.00	2	0.6	254	PASS
127	198	10	80	47.2	45648	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	96728	PASS
199	198	5	9	6.9	6712	PASS
275	198	10	60	26.4	25565	PASS
365	198	1	100	4.9	4783	PASS
441	198	0.01	100	10.0	9700	PASS
442	442	50	100	100.0	65680	PASS
443	442	15	24	17.3	11379	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
1/15/2025	BNA_N	<u>BN035925.D</u>
Compound Name	Response	Retention Time
DDT	350796	20.686
DDD	4625	20.298
DDE	0	19.748
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4625	355421	1.30

Instrument :
BNA_N
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011525\
Data File : BN035925.D
Acq On : 15 Jan 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 16 01:15:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

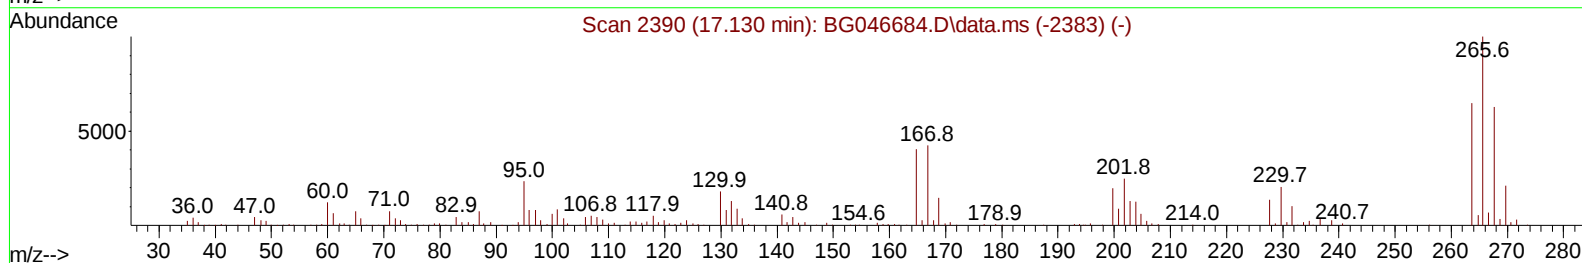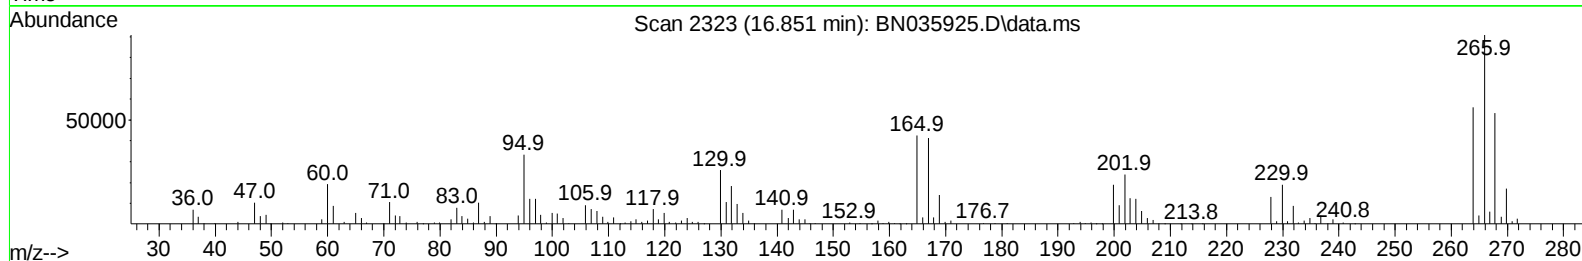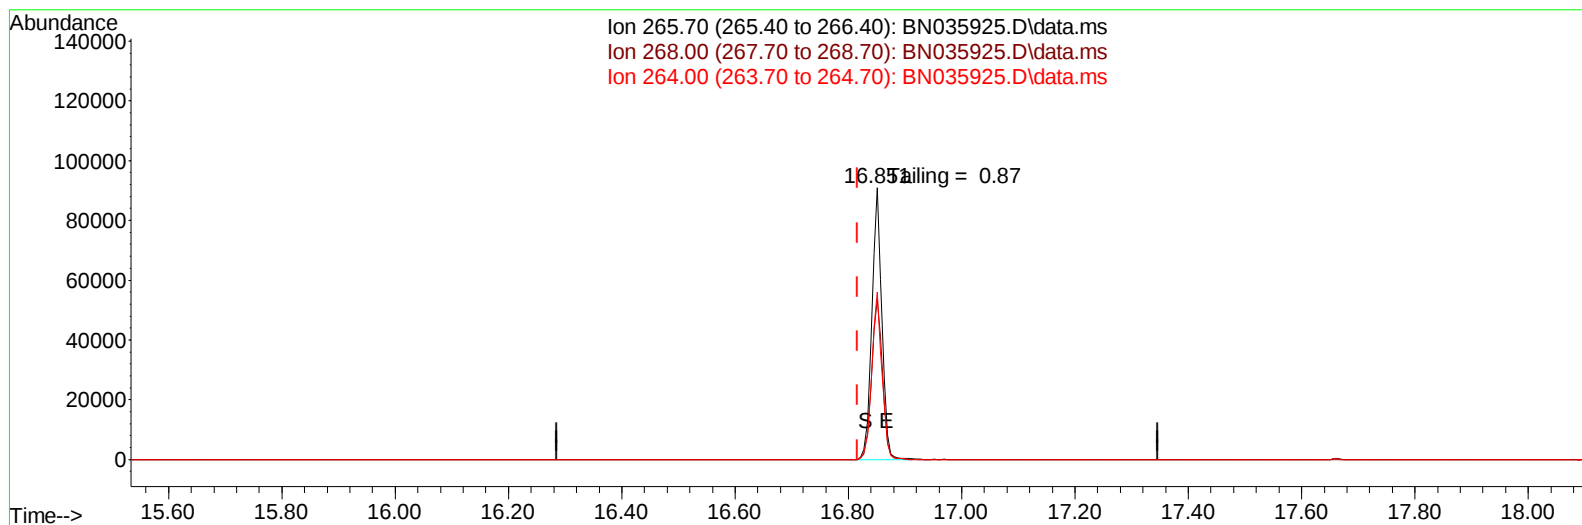

TIC: BN035925.D\data.ms

(70) Pentachlorophenol (C)

16.851min (+ 0.035) 20041.58 ng




response 111827

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	58.74
264.00	61.60	61.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011525\
Data File : BN035925.D
Acq On : 15 Jan 2025 09:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 16 01:15:22 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Dec 25 04:23:53 2024
Response via : Initial Calibration

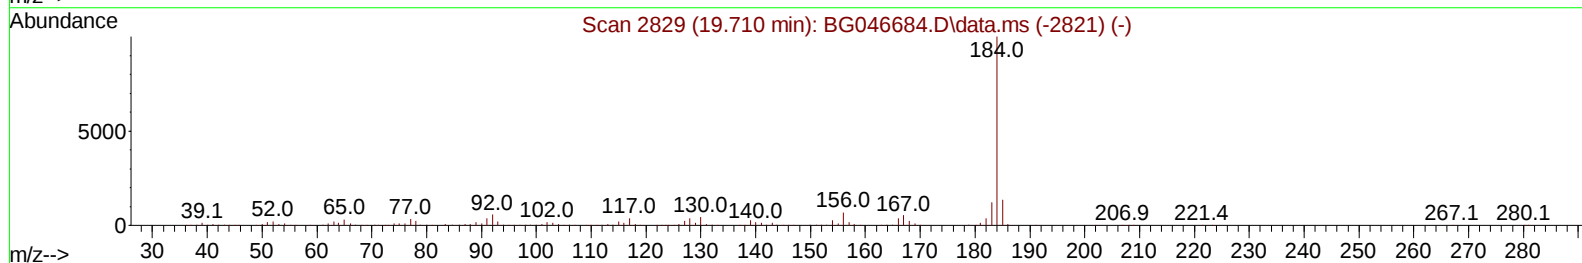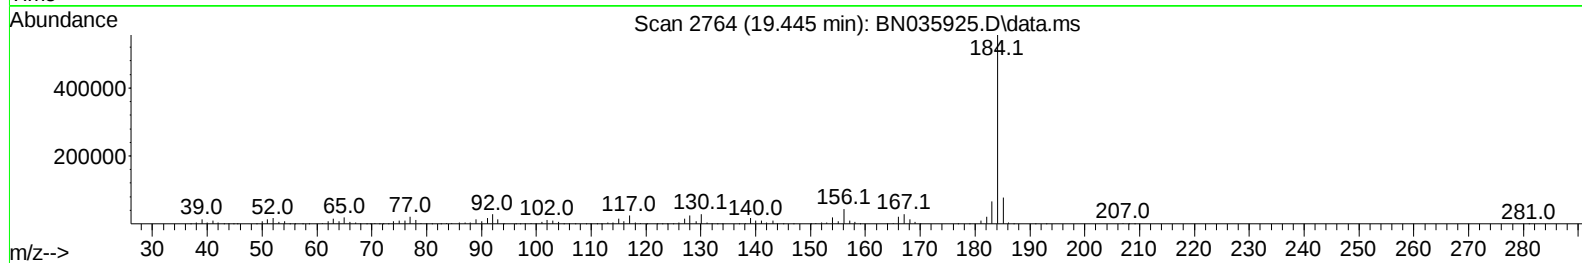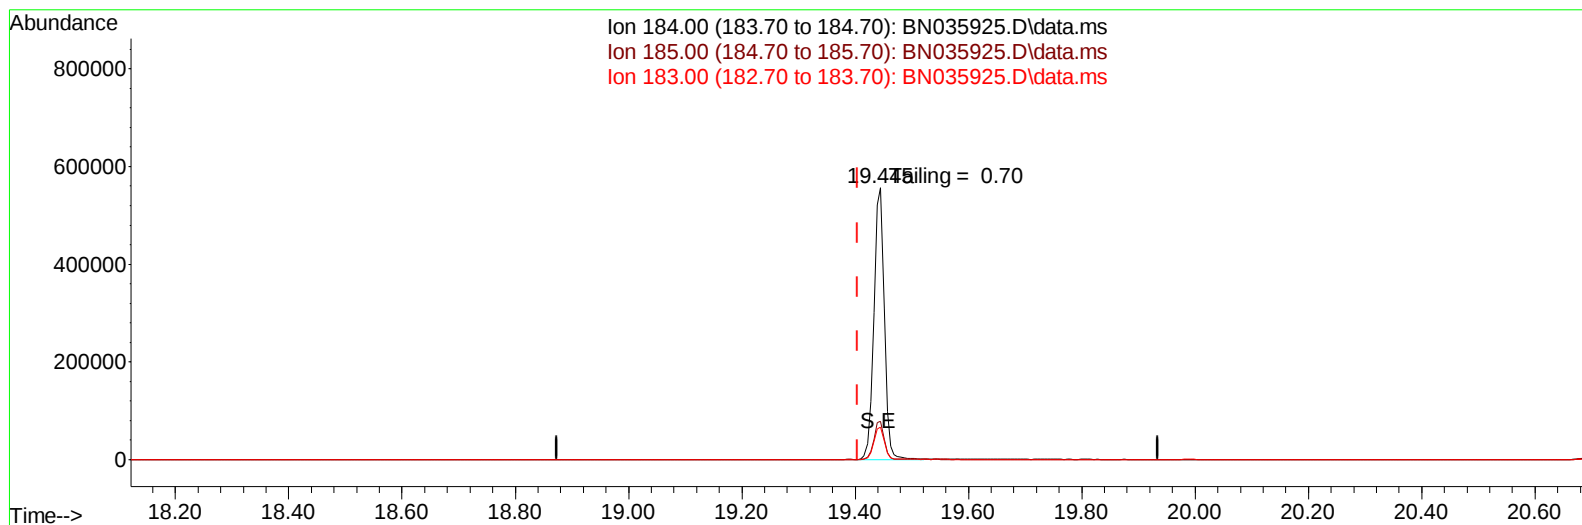

TIC: BN035925.D\data.ms

(77) Benzidine

19.445min (+ 0.041) 0.00 ng

response 709609

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.10
183.00	13.20	11.87
0.00	0.00	0.00