


Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM011620\
 Data File : BM024485.D
 Acq On : 16 Jan 2020 08:51
 Operator : JU
 Sample : DFTPP13
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM011520MA.M
 Title : SVOA CALIBRATION
 Last Update : Thu Jan 16 01:52:07 2020

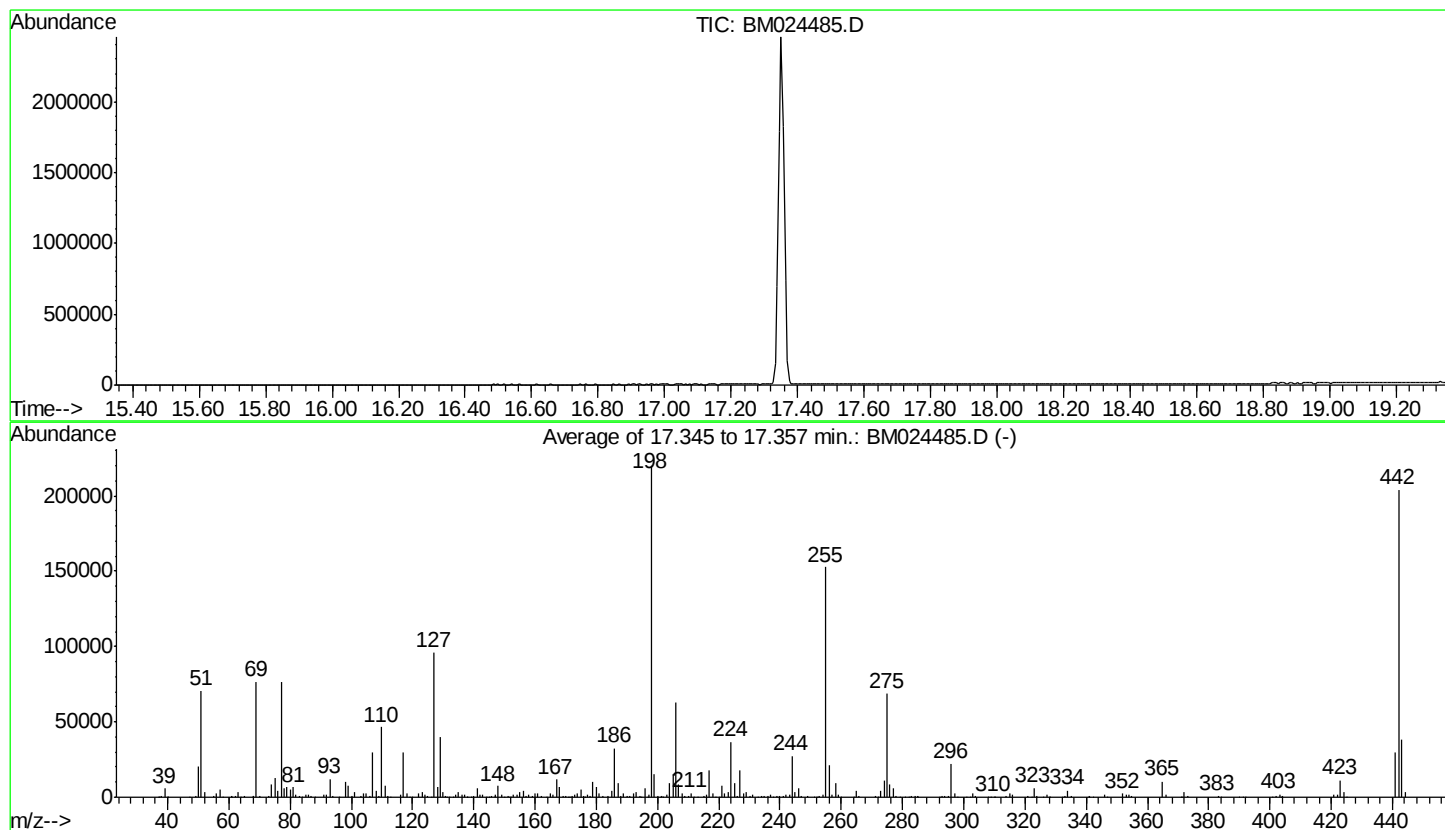

AutoFind: Scans 2458, 2459, 2460; Background Corrected with Scan 2453

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.2	70832	PASS
68	69	0.00	2	1.4	1093	PASS
69	198	0.00	100	34.8	76554	PASS
70	69	0.00	2	0.6	488	PASS
127	198	10	80	43.5	95720	PASS
197	198	0.00	2	0.6	1398	PASS
198	198	100	100	100.0	220074	PASS
199	198	5	9	6.9	15219	PASS
275	198	10	60	31.1	68549	PASS
365	198	1	100	4.7	10241	PASS
441	198	0.01	100	13.4	29560	PASS
442	198	50	100	92.8	204330	PASS
443	442	15	24	18.8	38480	PASS