


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN011620\
 Data File : BN009382.D
 Acq On : 16 Jan 2020 13:23
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN011420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 14 09:33:55 2020

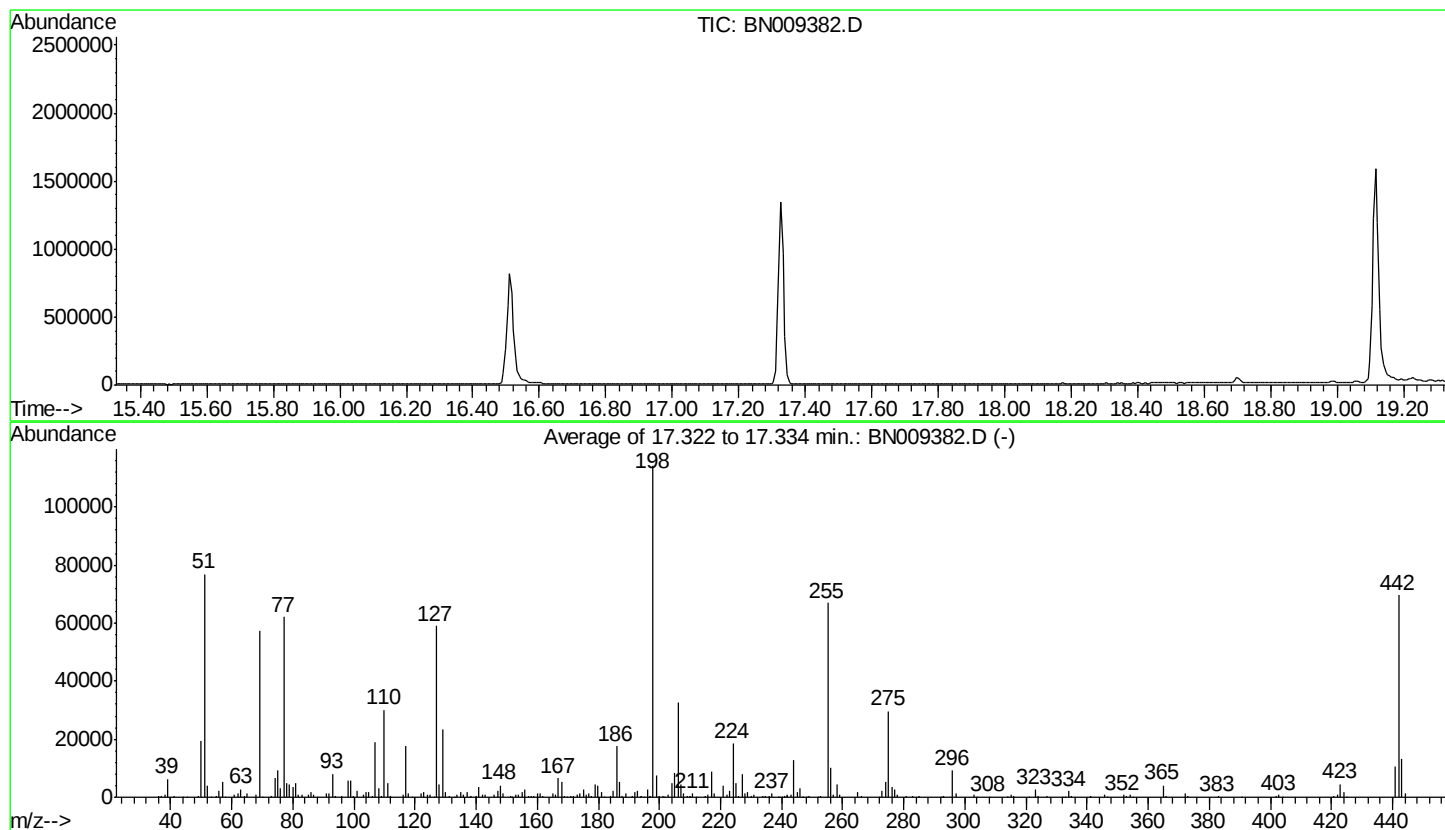

AutoFind: Scans 2437, 2438, 2439; Background Corrected with Scan 2431

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	67.3	76850	PASS
68	69	0.00	2	1.8	1032	PASS
69	198	0.00	100	50.4	57544	PASS
70	69	0.00	2	0.2	123	PASS
127	198	10	80	51.6	58928	PASS
197	198	0.00	2	0.5	515	PASS
198	198	100	100	100.0	114253	PASS
199	198	5	9	6.5	7431	PASS
275	198	10	60	25.9	29594	PASS
365	198	1	100	3.5	3980	PASS
441	198	0.01	100	9.4	10699	PASS
442	198	50	100	61.0	69640	PASS
443	442	15	24	18.7	13053	PASS