


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011623\
 Data File : BN023660.D
 Acq On : 16 Jan 2023 10:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN011223.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 17 13:44:46 2023

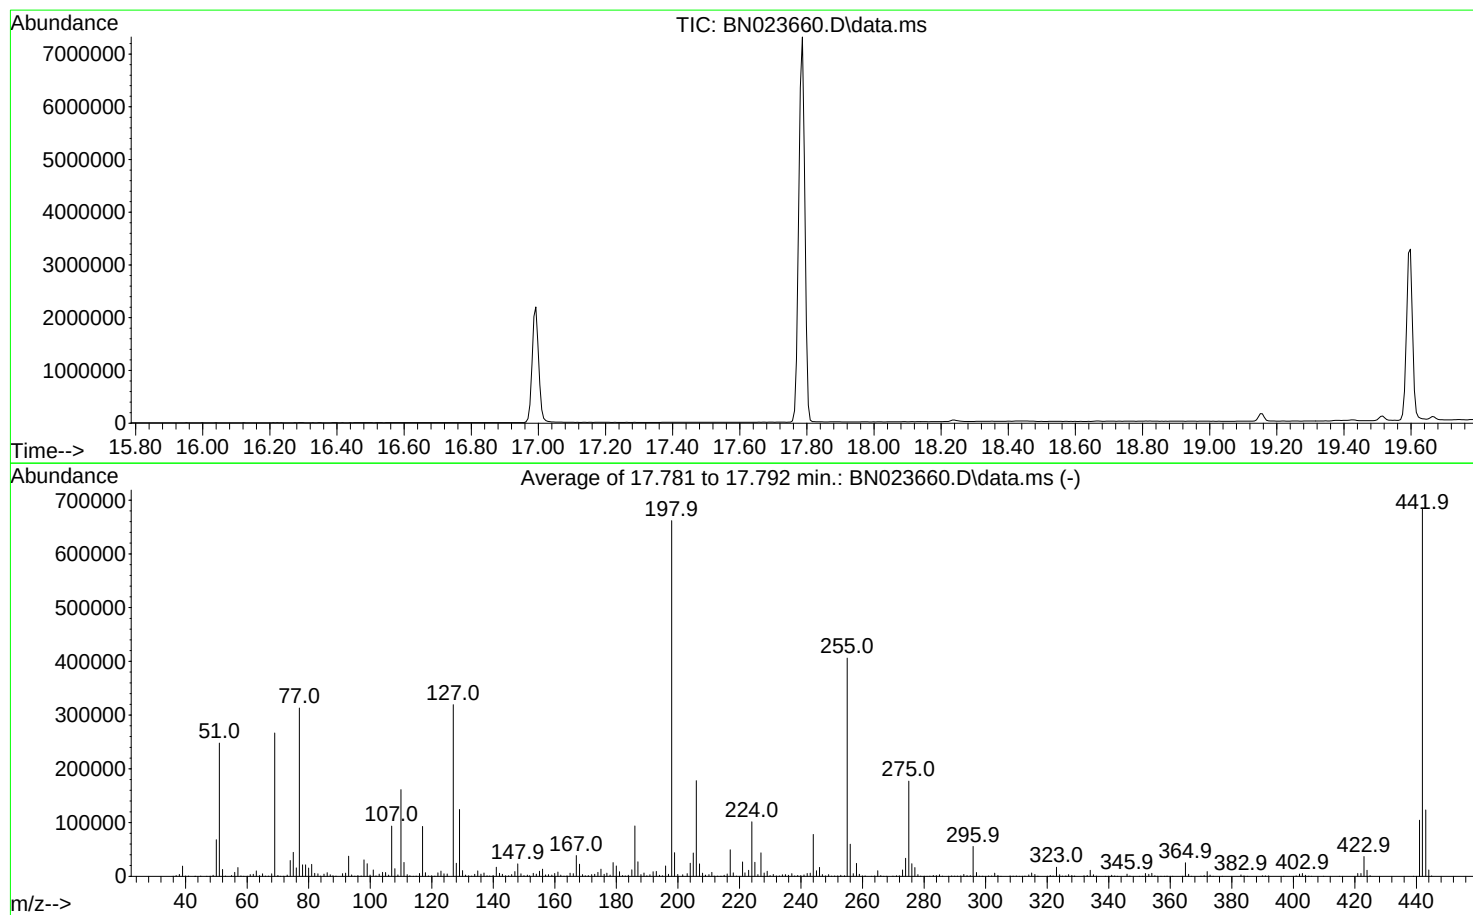




AutoFind: Scans 2498, 2499, 2500; Background Corrected with Scan 2490

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.5	248043	PASS
68	69	0.00	2	1.8	4761	PASS
69	198	0.00	100	40.3	266752	PASS
70	69	0.00	2	0.6	1551	PASS
127	198	10	80	48.3	319509	PASS
197	198	0.00	2	0.6	3812	PASS
198	198	100	100	100.0	661696	PASS
199	198	5	9	6.7	44021	PASS
275	198	10	60	26.8	177067	PASS
365	198	1	100	3.8	25195	PASS
441	198	0.01	100	15.8	104352	PASS
442	442	50	100	100.0	684608	PASS
443	442	15	24	18.0	123344	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011623\
Data File : BN023660.D
Acq On : 16 Jan 2023 10:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 17 08:00:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 08:00:23 2023
Response via : Initial Calibration

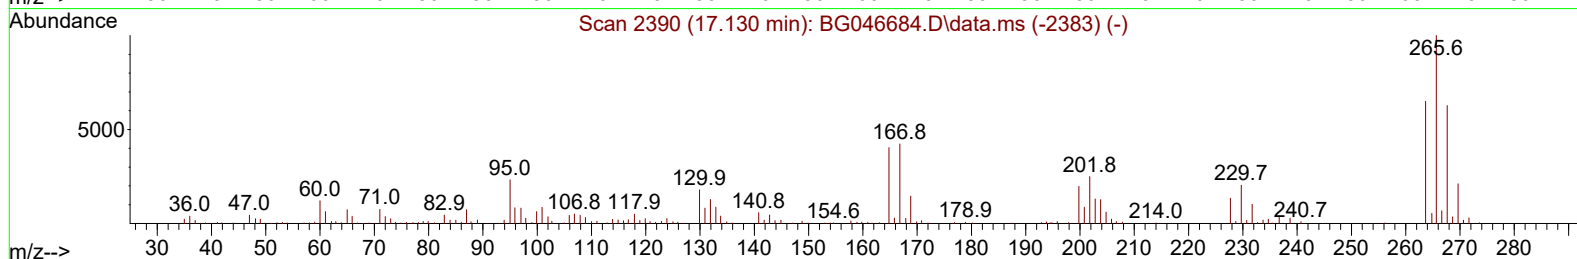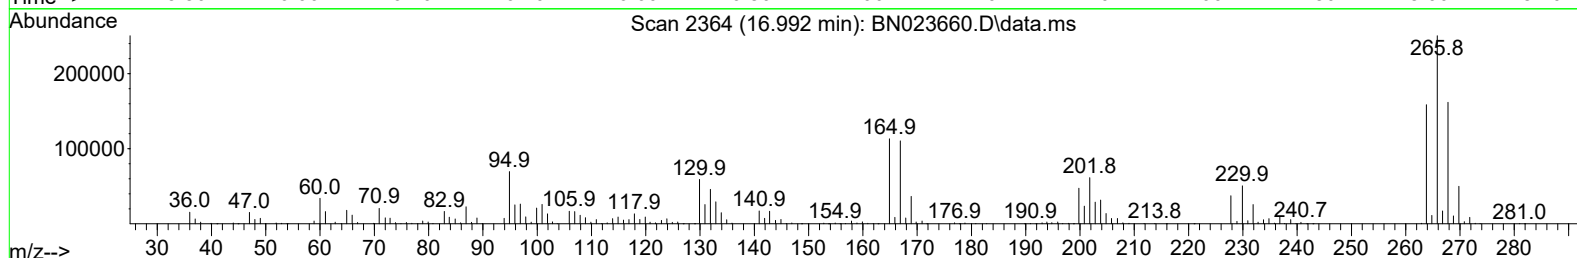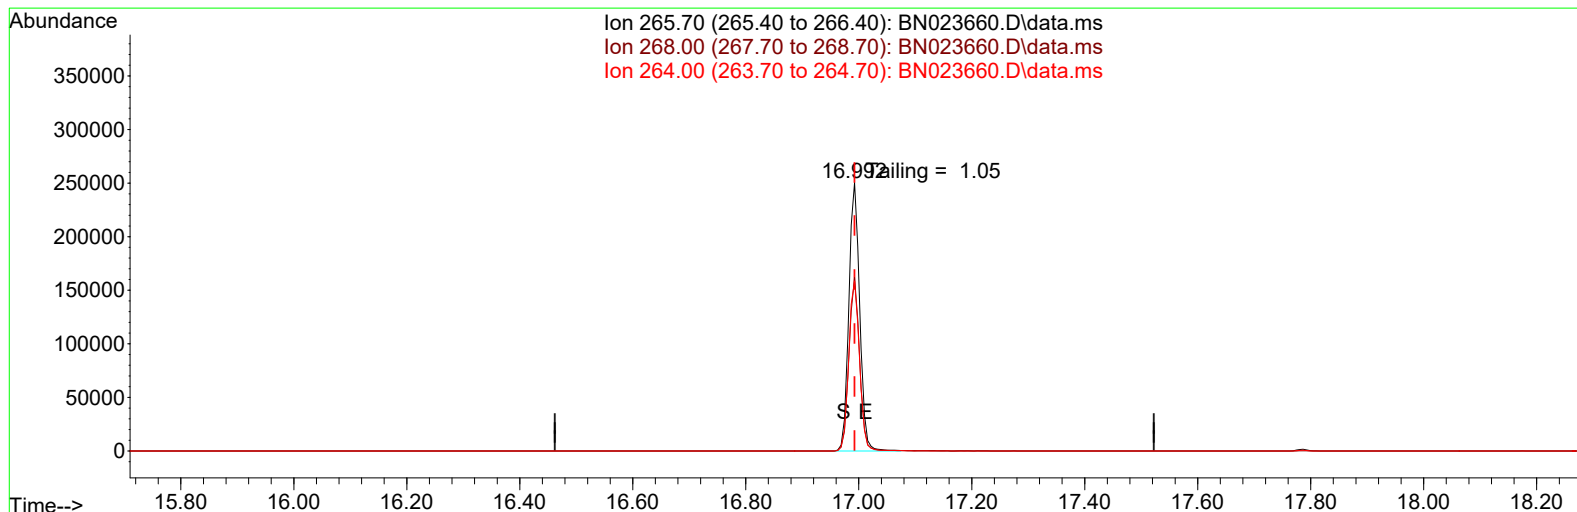

TIC: BN023660.D\data.ms

(70) Pentachlorophenol (C)

16.992min (0.000) 8752.27 ng




response 334705

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.58
264.00	61.60	63.38
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN011623\  
Data File : BN023660.D  
Acq On    : 16 Jan 2023  10:17  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jan 17 08:00:28 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 17 08:00:23 2023
Response via : Initial Calibration

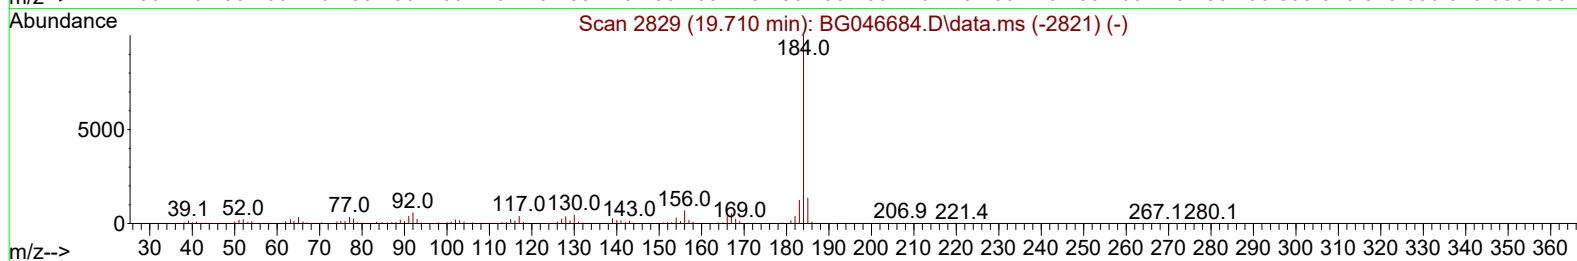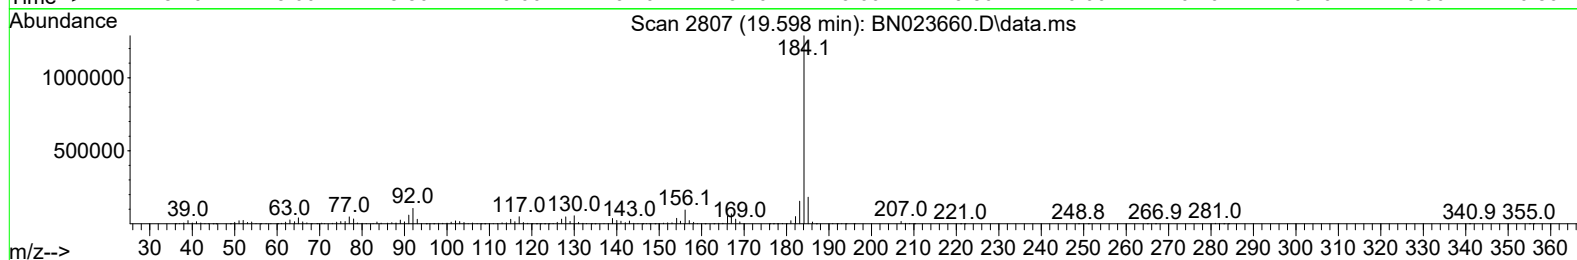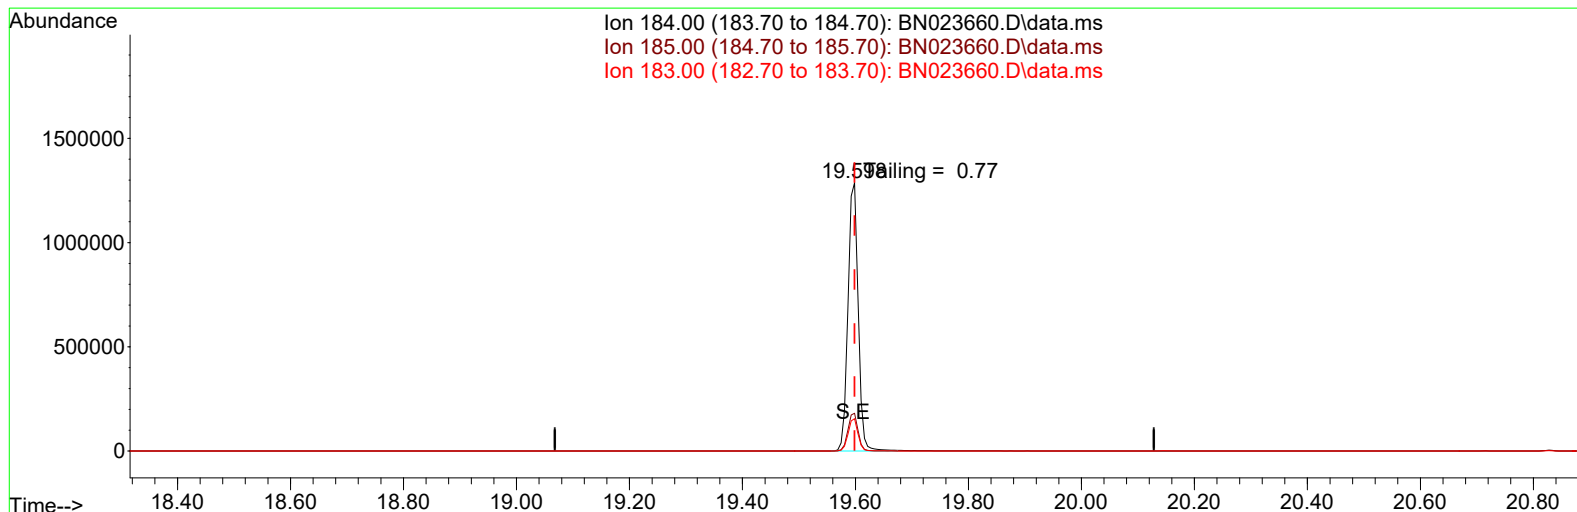

TIC: BN023660.D\data.ms

(77) Benzidine

19.598min (0.000) 0.00 ng

response **1622606**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.11
183.00	13.20	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/16/2023	BNA_N	<u>BN023660.D</u>
Compound Name	Response	Retention Time
DDT	896746	20.828
DDD	32291	20.386
DDE	1391	19.881
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
33682	930428	3.62

Instrument :
BNA_N
ClientSampleId :
DFTPP